



Warehouse Standard Operating Procedures

Federal Directorate of Immunization

Ministry of National Health Services,
Regulations and Coordination,
Government of Pakistan

DS WH-1



2023



Warehouse Standard Operating Procedures

Federal Directorate of Immunization

Disclaimer

This publication was prepared by the U.S. Agency for International Development (USAID) funded, Global Health Supply Chain Program – Procurement and Supply Management (GHSC-PSM) project, managed by Chemonics International Inc. The authors' views expressed in this publication do not necessarily reflect the views of the USAID or the United States Government.

USAID Pakistan Supply Chain Cooperation Standards and Policies can be found at:
<https://v.lmis.gov.pk/docs/pakistan-supplychain-sops>

CONTENTS

ACRONYMS vii

ACKNOWLEDGMENT..... ix

PREFACExi

INTRODUCTION 1

1.0 RECEIPT PROCEDURE..... 2

2.0 STORAGE11

3.0 ISSUE PROCEDURE.....16

4.0 DISPOSAL.....26

5.0 ANNEXURES28

ACRONYMS

AWB	Air Way Bill
BCG	Bacillus Calmette-Guérin
CCM	Cold chain monitoring
CR	Cold room
FDI	Federal Directorate of Immunization
FEFO	First to-Expire, First Out
FR	Freezer room
GHSC-PSM	Global Health Supply Chain Program-Procurement and Supply Management
Hib	Haemophilus Influenzae disease type b
ISO	Organization for Standardization
ILR	Ice-lined refrigerator
IRV	Issue and Receipt Voucher
MDVP	Multi-dose Vial Policy
MMR	Measles, mumps, rubella
MoNHSR&C	Ministry of National Health Services, Regulations & Coordination
OPV	Oral polio vaccine
PAD	Product Arrival Date
PAR	Product Arrival Report
PCV	Pneumococcal vaccine
SOP	Standard operating procedure
TT	Tetanus Toxoid vaccine
UN	United Nations
USAID	U.S. Agency for International Development
VAD	Vaccine Arrival Date
VAR	Vaccine Arrival Report
vLMIS	Vaccine logistics management information system
VVM	Vaccine vial monitor
WHO	World Health Organization
WMS	Warehouse Management System

ACKNOWLEDGMENT

Modernization of the central warehouse of Federal Directorate of Immunization (FDI), Ministry of National Health Services, Regulations, and Coordination, Islamabad has brought incredible results and has created the need for standardization to accelerate the pace of work. The scope and scale of work at the FDI warehouse in Islamabad have categorized it as the public institution for storing, managing, and distributing life-saving vaccines across the country. With the technical support of USAID funded Global Health Supply Chain Program – Procurement and Supply Management (GHSC-PSM) project, the FDI has been able to develop standard operating procedures (SOPs) for managing day to day operational activities at the central warehouse.

The FDI highly appreciates the valuable support extended by USAID/Pakistan towards sustainable immunization supply chain system strengthening in the country. We thank Mr. Bradley Cronk, Director Health Office, USAID/Pakistan for his leadership in successfully strengthening, rehabilitating, and upgrading the FDI Warehouse in Islamabad to improve warehouse management system as per the international standards.

We also express our gratitude to Dr. Muhammad Tariq, Country Director, USAID GHSC-PSM project in Pakistan, for his leadership role; and his dedicated team for their effort and support in developing the *Warehouse Standard Operating Procedures*.



Dr. Muhammad Ahmed Kazi
Director General,
Federal Directorate of Immunization, Islamabad

PREFACE

Standard operating procedures are crucial for the efficient and effective functioning of a vaccine warehouse. The aim of developing this document is to assist the FDI in optimizing vaccine inventory and cold chain management. The standard operating procedures will serve as a reference document for the FDI staff in ensuring the safety, quality, compliance, and efficiency of vaccine warehousing operations. The document provides a framework for consistency, mitigate risks, promote adherence to regulatory standards, and management of vaccines in the warehouse. The manual will play a crucial role in improving the vaccine logistics management system and properly organizing record keeping.

We would like to express our sincere gratitude to our colleagues and friends at USAID, both in Islamabad and Washington, who provided invaluable leadership support throughout this project. Special thanks to Mr. Bradley Cronk, Dr. Shabir Chandio, Mr. Khalid Mahmood, Mr. Sherif Mowafy, Mr. John Vivalo, Mr. Keith Hummel, and Mr. Ramy Guirguis for their contributions and dedication.

Together, we strive to improve vaccine logistics and contribute to a more efficient and effective healthcare service delivery system in Pakistan.

A handwritten signature in black ink, appearing to read 'Dr. Muhammad Tariq', is written over a horizontal line.

Dr. Muhammad Tariq

Country Director

USAID Global Health Supply Chain Program – Procurement and Supply Management

INTRODUCTION

Standard operating procedures (SOPs) are process document that detail how a worker should perform a given task and ensures that all storekeepers, workers, and laborers, under the supervision of the Store Officer and the Assistant Store Officer perform tasks in the same way, which will consistently produce the expected outcomes.

SOPs, used in combination with planned training and regular performance feedback, lead to an effective and motivated workforce.

This manual, *Warehouse Standard Operating Procedures*, will help operators and workers at the FDI Warehouse to streamline the vaccine logistics, supply chain, and inventory management.

All the staff must adhere to these SOPs in maintaining ISO certified environment for maintaining an International Organization for Standardization (ISO) certified warehousing environment including storage, distribution and inventory management.

ISO CERTIFICATION REQUIREMENTS AND PROCESSES

The ISO 9001:2008 requires a documented quality management system. General requirements include an organization to establish, document, implement, and maintain a quality management system and continually improve its effectiveness.

Quality management system documentation requires:

- Documented statements of a quality policy and quality objectives
- A quality manual
- Documented procedures
- Documents needed by the organization to ensure the effective planning, operation, and control of its processes
- Records

ISO 9001:2008 specifically requires the organization to have *documented procedures* for the following reasons:

- Control of documents
- Control of records
- Internal audit
- Control of non-conforming products
- Corrective action
- Preventive action

An ISO certification will not only ensure that quality is maintained within the premises, but also will establish credibility of its operations locally and internationally.

1.0 RECEIPT PROCEDURE

1.1 COLD STORE

1.1.1 RESPONSIBILITY

The Storekeeper, under the supervision of Store Officer/Assistant Store Officer, is responsible for receiving all the vaccines at the FDI Warehouse.

1.1.2 PROCEDURE FOR VACCINES PURCHASED FROM INTERNATIONAL RESOURCES

1.1.2.1 Pre-alert shipment intimation

- For vaccines purchased through the international sources, the FDI Warehouse must receive shipment pre-alerts and shipping documents by email or fax at least 10 days prior to the arrival. Documents will include:
 - ✓ Shipping information from procuring agency/freight forwarding agent ([Annex 1](#))
 - ✓ Copy of air way bill (AWB)- ([Annex 2](#))
 - ✓ Copy of packing list ([Annex 3](#))
 - ✓ Copy of invoice ([Annex 4](#))
 - ✓ Copy of release certificate ([Annex 5](#))
- Upon the arrival of advance intimations, delivery schedule for the Vaccine Arrival Date (VAD), storekeeper will check the documents, and will:
 - ✓ Check for availability of space and placement of incoming stock in the Freezer Room/Cold Room (FR/CR) of the Warehouse Management System/ vaccine logistics management information system (WMS/vLMIS)
 - ✓ Will record the flight arrival details in system as well as in shipping documents, record register and make arrangements for the collection of vaccine from the airport.
- Store officer will appoint a person who will deliver the shipment documents for the pre-appointed clearing agent at the port or airport for custom clearance.



- Will coordinate with the customs clearing agents and prepare the schedule for unloading, after consulting with them.

- Will confirm the readiness to receive vaccines by telephone or email if the airline requires doing so as a condition of delivery.
- Will arrange for the refrigerated trucks to be at the airport in time to collect the vaccine.

1.1.2.2 Collection of vaccine from the Airport

- Authorized clearing agent will clear the shipment through customs immediately after arrival of the flight and will deliver the shipment to FDI Warehouse preferably within six hours, but not later than 10 hours.
- Nominated FDI Warehouse person will transport the vaccine to the primary store by refrigerated vans and unload the vehicle immediately upon arrival.

1.1.2.3 Shipment inspection

- Before the inspection, the officer in-charge at the FDI Warehouse must ensure that all vaccines, including those received from international sources, are licensed for use in their country.
- The following documents that accompany the shipment must be checked:
 - ✓ Invoice
 - ✓ Packing list
 - ✓ Lot release certificate for the country of origin/Protocol Certificate ([Annex 6](#))
 - ✓ Vaccine Arrival Report (VAR)-([Annex 7](#))
- After the vaccines arrive at the FDI Warehouse, unload the refrigerated van, inspect the shipment, and check for physical damage or missing items.
- The following steps must be completed while inspecting the new shipment:
 - ✓ Count the packages according to the packing list
 - ✓ Segregate each batch of vaccine and diluents/droppers
 - ✓ Open each carton and stop the electronic shipping indicators (Data Loggers/Q-Tag or similar)
 - ✓ Check the vaccine vial monitor (VVM) status ([Annex 8](#)), and type and expiry dates for each type and batch of vaccine
 - ✓ Perform vaccine Shake Test ([Annex 9](#)) to determine whether the vaccine is frozen or not
 - ✓ Segregate ice packs/coolants from the vaccine and properly store them.
 - ✓ Dispose of dry ice, if received with stock
- Record the status of VVM stage, type, and expiry date of vaccine in the VAR.
Note: Do not record details of more than one vaccine type on a VAR. A separate VAR form must be completed for each vaccine—e.g., one for Oral Polio Vaccine (OPV), one for Bacillus Calmette-Guérin (BCG), etc.
- Check the status of the electronic shipping indicators. Record the details of any alarms on the Electronic Device Alarm Report form ([Annex 10](#))
- If there are no electronic shipping indicators, check the status of the cold chain monitoring (CCM) cards and record any color changes on the CCM card. Make a photocopy or scan the card; record the color change details and ensure its usability under the World Health Organization (WHO) and manufacturer guidelines.
- For diluents that accompany reconstituted vaccines, such as BCG or measles vaccine check the batch number, expiry date; and confirm that they comply with the order requirements.
- For droppers, in the case of oral polio vaccine, check a sample of the products to confirm that they comply with the order requirements.
- Record all other required details for each vaccine in the shipment on the VAR form supplied for that vaccine.

- Hand over a copy of the VAR to the procurement agencies office within 72 hours of the flight's arrival
- For each received shipment, of vaccine, a separate checklist is filled out for reporting and record keeping, as shown below:

Received Shipment Checklist

Date	Purpose	Antigen	Batch No	Manufacture	Received From

1.1.2.4 Stock placement

1.1.2.4.1 Vaccine accepted

If no problems are identified, and the vaccine is accepted, unpack the shipping containers and place the vaccine in the cold chain (FR/CR, refrigerator, or freezer). Place diluents in the diluent dry store. After physically stacking vaccines in the cold chain, enter the received vaccine quantity in the Stock Receive Form of the vLMIS as shown below, and place them into the designated FR/CR in the vLMIS, as already mentioned above.

Stock Receive (Supplier)

The following points must be filled in the Stock Receive Form of the vLMIS:

- Reference number
- Received from
- Purpose
- Name of vaccine/product
- Manufacturer of the vaccine
- Vial presentation (doses per vial)
- Batch number(s)
- Expiry date
- Quantity of vials received
- VVM type
- VVM stage
- Name of cold chain equipment where the vaccine is kept

1.1.2.4.2 Vaccine rejected

- In case of unusable VVM stage and type or expired vaccine, and if problems or discrepancies are identified, immediately report the concerns to the supplier representative. If issues are identified, do not unpack the vaccine until the issue is resolved.
- Till reaching the resolution, stack the affected shipping container(s), with the temperature monitoring device(s), in holding area of designated FR/CR, as appropriate. Clearly mark each container "DO NOT USE." Place any associated diluents in a designated area of the diluent dry store.
- DO NOT record the arrival in the vLMIS.
- The storekeeper will retain VARs and all correspondence relating to the unsatisfactory shipments or procedures for a minimum period of 5 years.

1.2 VACCINE INVENTORY MANAGEMENT

1.2.1 RESPONSIBILITY

The storekeeper under the supervision of the Store Officer/Assistant Store Officer is responsible for the vaccine inventory management.

1.2.2. PROCEDURE

- Ensure that all receipts and the dispatched transaction of the vaccine stocks are recorded in the WMS/vLMIS or in the stock register, daily.
- No transactions can be made outside the vLMIS and no supplies can leave the store without an Issue and Receipt Vouchers (IRVs) generated by the vLMIS.
- Ensure that full details of all transactions are completely entered immediately, as they occur.
- To identify the status of inventory for each vaccine, ensure that all vaccine stock has stock cards and bin cards updated and placed in front of each vaccine lot or batch.
- Physically compile and reconcile the dispatched and received vaccine stock in the FDI Warehouse with the quantities reflected in the WMS/vLMIS or stock register.
- Ensure that the vaccine commodities information on the WMS/vLMIS, or stock register, reconciles with the physical stock, location, rack, and pallet.
- Physically monitor and check all vaccines for the name, location, rack, pallet, lot, and batch; and ensure they are correctly identified in the WMS/vLMIS or stock register.
- Identify and correct any incorrect entries in the FR/CR location, rack, and pallet, and in all areas of the warehouse.
- Manually prepare and record the dispatched and received vaccine commodities on a daily basis and report it in the WMS/vLMIS or in the stock register.
- Stock records, such as IRVs must be up to date in the vLMIS. Data files must be backed up daily and the backup media must be kept in a safe place.
- To obtain prints of the vaccine stock sufficiency reports and reviews, have the relevant FDI Warehouse authority sign them and file them.
- Identify and take precautionary measures to safeguard vaccine stock from loss, theft, damage, and expiry.
- Ensure that all features of the WMS /vLMIS are working appropriately and are error free and that any problems that occur with the WMS/vLMIS are reported immediately.
- Ensure that all the WMS/vLMIS equipment is running smoothly, and that it is kept and maintained in good condition.
- Ensure that all vaccine commodities placed in the FDI Warehouse are scanned and arranged by location in each FR/CR.
- Ensure that the vaccine and supplies commodities are released based on the First to Expire, First-Out (FEFO); and that any short expiry is reported immediately to management.

1.3 DRY STORE

1.3.1 RESPONSIBILITY

The Storekeeper, under the supervision of the Store Officer/ Assistant Store Officer, is responsible for receiving all ancillary supplies at the FDI Warehouse. Supplies in dry store contain syringes, safety boxes, vitamin capsules, refrigerators, freezers, cold boxes, and vaccine carriers etc.

1.3.2 PROCEDURE

1.3.2.1 Shipment Pre-alert

- The FDI Warehouse must receive pre-alert shipment intimation and documents by 10 days before the arrival of supplies.
- Get delivery schedule for Product Arrival Date (PAD); and prepare proper logistics and administrative arrangement in advance.
- Check available space and plan placement of incoming stocks and update in the vLMIS as shown below:

WELCOME

Userrep1

Dashboard

Inventory Management

Stock Placement

Manage Location

Location Status

Manage Gatepass

Cold Chain

Reports

CCEM Reports

Maps

Inventory Graphs

CCEM graphs

Campaign Reports

Location Status

Dry Store Locations

Cold Store Locations

Store1

RowA

Show Status

1A1A1	1A1A2	1A2A1	1A2A2	1A3A1	1A3A2	1A4A1	1A4A2	1A5A1	1A5A2	1A6A1	1A6A2
1A1A3	1A1A4	1A2A3	1A2A4	1A3A3	1A3A4	1A4A3	1A4A4	1A5A3	1A5A4	1A6A3	1A6A4
1A1A5		1A2A5		1A3A5		1A4A5		1A5A5		1A6A5	
1A1B1	1A1B2	1A2B1	1A2B2	1A3B1	1A3B2	1A4B1	1A4B2	1A5B1	1A5B2	1A6B1	1A6B2
1A1B3	1A1B4	1A2B3	1A2B4	1A3B3	1A3B4	1A4B3	1A4B4	1A5B3	1A5B4	1A6B3	1A6B4
1A1B5		1A2B5		1A3B5		1A4B5		1A5B5		1A6B5	
1A1C1	1A1C2	1A2C1	1A2C2	1A3C1	1A3C2	1A4C1	1A4C2	1A5C1	1A5C2	1A6C1	1A6C2
1A1C3	1A1C4	1A2C3	1A2C4	1A3C3	1A3C4	1A4C3	1A4C4	1A5C3	1A5C4	1A6C3	1A6C4
1A1C5		1A2C5		1A3C5		1A4C5		1A5C5		1A6C5	

- The following must be checked in the shipment, pre-alert documents:
 - ✓ Shipping notification from freight forwarding agent to concerned FDI Warehouse staff.
 - ✓ Copy of packing list ([Annex 12](#))
 - ✓ Copy of invoice ([Annex 13](#))
- Check these documents and file them in the product arrival file.
- FDI Warehouse concerned authorities will deliver the shipment documents for the pre-appointed clearing agent at the port or airport for custom clearance.
- Closely coordinate with the customs clearing agent and prepare the schedule for unloading.

1.3.2.2 Collect Shipment from the Port of Entry

- Clear the shipment through customs within maximum allowable period preferably less than 24 hours of flight arrival.
- Transport the products to the store or warehouse and immediately unload the vehicle.

1.3.2.3 Shipment Inspection

- Inspect the shipment when it arrives at the FDI Warehouse and check for physical damage or missing items.
- Check following documents accompanying the shipment;
 - ✓ Invoice
 - ✓ Packing list
 - ✓ Certificate of conformity ([Annex 14](#))
 - ✓ Copy of Product Arrival Report (PAR) ([Annex 15](#))
- Syringes: Check the lot numbers, expiry dates, and/or manufacturing dates and confirm that they comply with the order requirements
- Safety boxes: Check a sample of the products to confirm that they comply with the order requirements.
- Vitamin A capsules: Check the batch numbers, and manufacturing and expiry dates, and confirm that they comply with the order requirements.
- Single-use electronic devices: This category includes freeze indicators and 30-day refrigerator temperature loggers. Check the lot numbers, expiry dates, and/or manufacturing dates; and confirm that they comply with the order requirements.
- Refrigerators and freezers: Check that the model numbers comply with the order requirements and that all loose components, such as vaccine baskets and spare parts, have been supplied.
- Cold boxes and vaccine carriers: Check that the model numbers comply with the order requirements and that the correct number and type(s) of water packs have also been supplied.
- Record all required details for each product in the Product Arrival Report (PAR).
- If no problems are identified and the products are accepted, transport them to the correct store or warehouse.
- If problems are identified, stack the unopened shipment on pallets or shelves in a designated area. Clearly mark the shipment "DO NOT USE."
- If problems have been reported, the Storekeeper will carry out follow-up activities, as agreed with supplier/procuring agent.

Received Shipment Checklist

Date	Purpose	Item	Batch No	Manufacturer	Received From

1.3.2.4 Stock placement

1.3.2.4.1 Shipment accepted

If no problems are identified and the product(s) are accepted, stock them in the correct store/location.

1.3.2.4.2 Shipment rejected

Any problems/ discrepancy/rejection due to damage/non- conformance with shipping documents should be immediately brought to the attention of the procuring agency through the FDI. Do not merge the disputed stock with the active inventory until a final decision is reached.

- Stack the unopened shipment on pallets or shelves in a designated area. Clearly mark the shipment “DO NOT USE.”
- Retain PARs and all correspondence relating to unsatisfactory shipments or procedures for a minimum of 5 years.

1.3.2.5 Stock Received in vLMIS

1.3.2.5.1 Syringes and safety boxes

- After receiving and unpacking the entire stock, physically place all the stock in their respective racks, pallets, and bins.
- Correctly enter the received stock into stock using the Stock Receive form of the vLMIS, as shown below and place them into the designated Dry Store Location in the vLMIS as already mentioned above.

Stock Receive (Supplier)

Fill out this form

Receipt No.	Ref No. *	Received From (Funding Source)*	Received Time
		GA/I	23/01/2023 04:30 PM
Purpose *	Product *	Used for	Manufacturer *
Routine	AD Syringe 0.5ml		Select
Batch No. *	Production Date	Expiry Date *	Unit Price per dose (PKR) *
Quantity *	Placement Location *		
	1A1A1		
Pcs			

Add Stock Receive

1.3.2.5.2 Refrigerators, freezers, vaccine carriers, and cold boxes:

Record the arrival in the stock control system, including manufacturer's name, model, and serial number. Record the required product details in the national cold chain equipment inventory.


EPI
 Information Management Systems


Vaccine (vLMIS)
 Pakistan Logistics Management Information System


 EPI
 Directory


 Training
 Manuals


 Home

ccem_national ▾

WELCOME
 Ccem_national

Dashboard
 Cold Chain
 Search Refrigerator
 Add Refrigerator
 Search Vaccines Carriers
 Add Vaccines Carriers
 Search Ice Pack
 Add Ice Pack
 Search Cold Room
 Add Cold Room
 Add Voltage Regulator
 Search Voltage Regulator
 Search Generator
 Add Generator
 Search Transport

Cold Chain

Search Refrigerator/Freezer/ILR Asset

Asset Sub Type Select Asset Sub Types	Source of Supply Select Source Of Supply	Working Status Select working status	Asset Id / Equipment Code
Catalogue ID 	Make Select Makes	Model Select Make First	Serial Number
Gross Capacity From 	Gross Capacity To 	Working Since From 	Working Since To
Placed At ☒ Select Warehouse ☐ Unallocated			
Office * Federal	Warehouse Federal Vaccine Store		

Search
 Reset

2.0 STORAGE

2.1 COLD STORE

2.1.1 RESPONSIBILITY

The Storekeeper under the supervision of the Store Officer/Assistant Store Officer is responsible for the storage of vaccines and supplies at the cold and dry stores at the FDI Warehouse.

2.1.2 PROCEDURE


- Remove the primary packings of vaccine from cartons and place them in the FR/CRs.
- Store ice packs or coolants received in the FR/CRs.
- Clean soiled or dusty exteriors of cartons before placing those in the stores and/or FR/CRs.
- Place the different vaccines in the FR/CRs in an appropriate space between each inner box, block, or tray of vaccine, which will allow the cold air to circulate around the vaccine.
- Store vaccines that have similar packaging in different locations in the cold/refrigerator rooms to avoid confusion and medication errors.
- Place the heat sensitive vaccines in the freezer rooms and other vaccines in the cold rooms.
- Do not place the freeze sensitive vaccines in freezer rooms.
- Vaccines for reconstitution can be placed in both the FR/CRs.
- Place each vaccine carton on the allocated shelf in the FR/CR's lot wise.
- Vaccines stored on pallets or racks should be free from moisture, dirt, insect, or rodent contamination.
- Clean up broken or spoiled product in a timely manner.
- Place proper tags on the vaccines shelves and racks including information on vaccine name, manufacturer, purpose, expiry date, and vaccine arrival date.
- Clearly label with the specific vaccine name, the location of each specific vaccine inside the cold/refrigerator or the storage unit room.
- Inspect that the cold chain equipment is functioning correctly; if any problem is noticed, immediately inform the cold chain mechanical engineer.
- Using the vaccines repacking protocols, repair and repack damaged cartons of vaccines before they are placed in the cold/refrigerator rooms. Rotate vaccine stock once a week; place them in the FR/CRs based on the expiration date, once a week and every time a new vaccine shipment arrives.
- Set the temperature alarms in the cold/refrigerator rooms; update the temperature logs daily.
- On a daily basis, randomly check the quality of the vaccines, or do a vaccine Shake Test of the suspected batch or lot.
- Disinfect and spray the storage area every third month against insects, rodents, and harmful bacteria, which are threats to the dry supplies and the health of the staff.
- Place and update the vaccine tags located in the appropriate FR/CR any time the status of stocks changes.
- Perform a physical count periodically—monthly, quarterly, and annually—to detect discrepancies.
- Restrict access to storage areas for vaccines to authorized personnel only.

- Record the FR/CR temperature on the logbook or chart twice a day to verify that the storage temperature is within the acceptable temperature ranges of +2°C to +8°C in cold rooms and vaccine refrigerators and -25°C to -15°C in the freezer room and freezers.
- This temperature chart also helps detect temperature alarm conditions that may cause vaccine damage and allows appropriate action to be taken; to assess the performance, over time, for vaccine handling at each link of the cold chain; and to monitor the performance of cold chain equipment.
- A temperature chart for FR/CRs is shown below:

Temperature Chart

Date	AM	°C	Initial	PM	°C	Initial

After receiving stock, both physically and in the vLMIS, locate/place the received stock into the designated CRs/FRs of the vLMIS, as shown below:

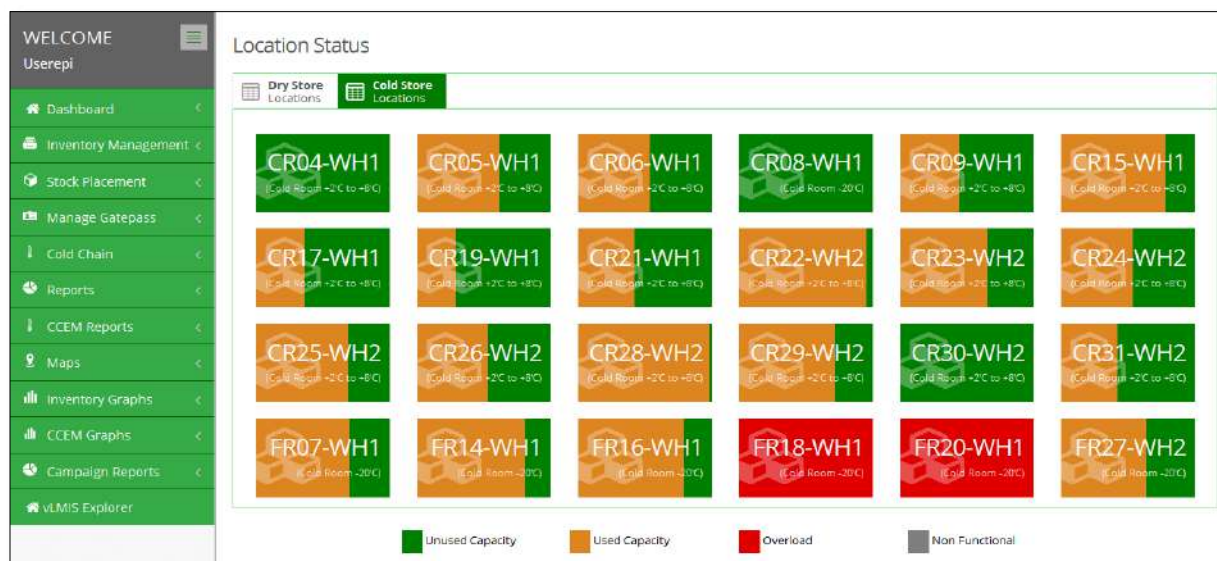

By clicking on the required FR/CR, stock can be placed, as shown below:

Back to Location								
25	records per page							
S.No.	Product	Batch No.	Expiry Date	Qty (Vials)	Qty (Doses)	VVM Stage	Action	
1	IPV	V0E071V	31/03/24	350	3,500	Usable	Transfer	Q
2	IPV	V0D141V	29/02/24	2,000	20,000	Usable	Transfer	Q
3	IPV	V0E051V	29/02/24	4,330	43,300	Usable	Transfer	Q
4	IPV	V0E491V	31/03/24	320	3,200	Usable	Transfer	Q
5	Measles Rubella-10VR Routine	0120V170	31/10/23	1,000	10,000	1	Transfer	Q
6	Measles Rubella-10VR Routine	0120V166	31/10/23	90	900	1	Transfer	Q
7	Pentavalent-1	68V01000	31/12/24	73,110	73,110	1	Transfer	Q
8	Pentavalent-1	220103822A	30/11/24	101,370	101,370	1	Transfer	Q
9	TCV (Routine)	70E22009A	29/02/26	2,073	16,385	1	Transfer	Q
10	TCV (Routine)	70E22013A	31/03/26	21,666	169,720	1	Transfer	Q
11	TCV (Routine)	70E21013A	29/02/24	21,610	169,200	1	Transfer	Q

Showing 1 to 11 of 11 entries

By clicking on transfer button, stock can be transferred from one bin to another, as shown below:

WELCOME Userop

Stock in Bin -

Transfer Stock from: CR19-WH1

Product: Measles-10 Batch No.: 004M41318 VVM Stage: 1 Available Quantity: 15900

Location: Select Location Quantity:

Transfer

Showing 1 to 4 of 4 entries

2.1.3 STORAGE OF SHIPMENT CHECKLIST

A checklist for storing a shipment of vaccine received is shown below:

Storage													
Is Data Logger available & functional?	Are Ice Packs available?	Are Coolant available?	Is Stock received according to prescribed alert?	VVM Stage	VVM Type	Expiry Date	Total Ice Pack Per Carton	Total Primary Boxes Per Secondary Box	Total Vials Per Primary Box	Total Secondary Boxes Per Carton	Total Vials Per Secondary Box	Total Vials Per Carton	Cold Room Number/ Freezer Number in which vaccines are placed

- Place and store the diluents and droppers accompanying the vaccine shipments in the designated bins of the racks in the dry warehouse at room temperature.
- Correctly place and enter the quantities of diluents and droppers on their respective bins in the WMS/vLMIS, as placed in the warehouse.

2.2 DRY STORE

After receiving stock, both physically and in the vLMIS, locate/place the received stock into the designated bins, pallets, and racks of the vLMIS, as shown below:

WELCOME

Location Status

Dry Store Locations Cold Store Locations

Store: 1 Row: A

Show Status

1A1A1	1A1A2	1A2A1	1A2A2	1A3A1	1A3A2	1A4A1	1A4A2	1A5A1	1A5A2	1A6A1	1A6A2
1A1A3	1A1A4	1A2A3	1A2A4	1A3A3	1A3A4	1A4A3	1A4A4	1A5A3	1A5A4	1A6A3	1A6A4
1A1A5		1A2A5		1A3A5		1A4A5		1A5A5		1A6A5	
1A1B1	1A1B2	1A2B1	1A2B2	1A3B1	1A3B2	1A4B1	1A4B2	1A5B1	1A5B2	1A6B1	1A6B2
1A1B3	1A1B4	1A2B3	1A2B4	1A3B3	1A3B4	1A4B3	1A4B4	1A5B3	1A5B4	1A6B3	1A6B4
1A1B5		1A2B5		1A3B5		1A4B5		1A5B5		1A6B5	
1A1C1	1A1C2	1A2C1	1A2C2	1A3C1	1A3C2	1A4C1	1A4C2	1A5C1	1A5C2	1A6C1	1A6C2
1A1C3	1A1C4	1A2C3	1A2C4	1A3C3	1A3C4	1A4C3	1A4C4	1A5C3	1A5C4	1A6C3	1A6C4
1A1C5		1A2C5		1A3C5		1A4C5		1A5C5		1A6C5	

By clicking on the required bin, stock can be placed, as shown below:

WELCOME

Stock in Bin - 1A1A1

Back to Location


10 records per page

Place More

Product	Batch No.	Carton Quantity	Quantity	Action
AD Syringe 0.5ml	0915/07		24	31200 Transfer

Showing 1 to 1 of 1 entries

By clicking on transfer button, stock can be transferred from one bin to another, as shown below:

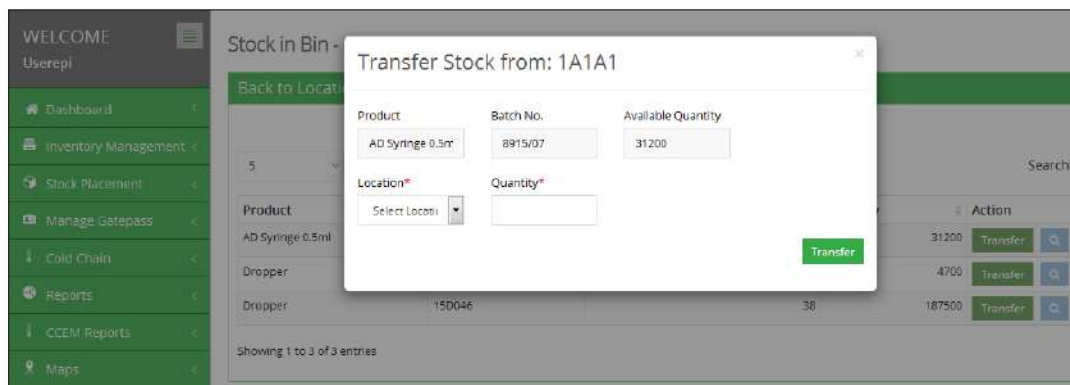

- All products are safely stored within the temperature and humidity levels specified for the product type.
- Access to storage areas—including products, packaging materials, and exterior storage areas—must be restricted to authorized personnel only.
- Store diluents, syringes, and other products with a limited shelf life in a separate location so they can easily be located and distributed in FEFO order.
- Store products without an expiry date, such as safety boxes, in a separate location so they can easily be located and distributed in FEFO order.
- Keep expired or damaged products marked for disposal separate from usable stock.
- Using the supplies repacking protocols, repair and repack damaged cartons of dry supplies before they are placed on the racks and pallets in the dry store.
- Rotate stock once a week, based on the expiration date and every time a new shipment arrives.
- Use proper stackers to place pallets in the allocated racks or area; ensure that cartons or pallets are not leaning over the edge of the racks or shelves.
- Maintain pallets, racks, and equipment in good condition to prevent any physical damage to materials or products (e.g., free from nails, wood splinters etc.).
- Keep the dry storage area clear and clean; keep the aisles empty to enable the stacker to operate and to allow people to walk through.
- Randomly check the quality of the dry store supplies daily.
- Disinfect and spray the storage area every third month against insects, rodents, and harmful bacteria, which are threats to the dry supplies and the health of the staff.
- Use stackers to place pallets on the racks.
- Place and update the diluent bin cards in the dry warehouse any time the status of stocks changes.
- Do a physical count periodically—monthly, quarterly, and annually—to detect discrepancies.
- Place received refrigerators or ice-lined refrigerators (ILRs), vaccine carriers, and cold boxes in the dry warehouse of the FDI Warehouse.
- Ensure that the dry supplies carton is secure and properly packed on all sides.

3.0 ISSUE PROCEDURE

3.1 COLD STORE

3.1.1 RESPONSIBILITY

The Storekeeper under the supervision of the Store Officer/Assistant Store Officer is responsible for issuing vaccines and supplies to provinces and districts at the FDI Warehouse.

3.1.2 PROCEDURE

- Acquire the complete signed requisition/demand of vaccines from all provinces, including the public- and private-stakeholders.
- Relevant officials of FDI will review and analyze the vaccine requirements for each stakeholder; to fulfill the requirement against the availability of vaccine stock in the FDI Warehouse.
- Approval sheet, or the release order request, for the requested vaccines will be shared with store officials.
- The approval sheet should contain the essential information, including the quantity requested by the province and district and the current stock status at the FDI Warehouse.
- The approval sheet for the resale of vaccines will include a recommendation to decrease the number of vaccines based on the actual demand by clients, after a stock sufficiency analyses.
- Vaccines will be issued to all province stakeholders that maintain the minimum/maximum level of vaccine stock at the FDI Warehouse.
- Prepare the vaccine dispatch order sheet/release order that has all the necessary information related to the requested vaccines.
- Generate the electronic vaccine picking list/priority vaccine distribution list from the vLMIS, as shown in the figure below:

Priority Vaccines Distribution

					Summary	Detail
Product	Batch Number	Expiry Date	VVM	Cold room	Quantity (Vials)	Quantity (Doses)
Priority 2						
sOPV (Campaign)	U9P811V	Nov. 2023	Usable	FR18-WH1	15,000	301,000
Total:					15,000	301,000
Priority 3						
sOPV (Campaign)	202202008	Feb. 2024	Usable	FR14-WH1	3,511	72,220
sOPV (Campaign)	202202011	Feb. 2024	Usable	FR14-WH1	1,820	32,400
sOPV (Campaign)	ACP46710AA	Mar. 2024	Usable	FR35-WH1	10,000	206,000
sOPV (Campaign)	U9F721V	Apr. 2024	Usable	FR20-WH1	11,948	239,000
sOPV (Campaign)	2042322	May. 2024	Usable	FR44-WH2	800	16,000
sOPV (Campaign)	ACP46720AA	May. 2024	Usable	FR40-WH2	188,042	3,138,040
sOPV (Campaign)	ACP46721AA	Jun. 2024	Usable	FR34-WH1	22,200	444,000
Total:					216,919	4,338,380
Priority 2						
Measles Rubella-10(MR Routine)	0120V099	Jul. 2023	1	CR41-WH1	181	1,010
Measles Rubella-10(MR Routine)	0120V138	Sep. 2023	1	FR22-WH1	2,340	23,600
Measles Rubella-10(MR Routine)	0120V140	Sep. 2023	1	CR45-WH2	300	3,000
Measles Rubella-10(MR Routine)	0120V179	Oct. 2023	1	FR07-WH1	1,200	12,000
Measles Rubella-10(MR Routine)	0120V171	Oct. 2023	1	CR08-WH1	8,800	88,000
Measles Rubella-10(MR Routine)	0120V175	Oct. 2023	1	CR22-WH2	1,500	15,000

- For vaccines going by air, calculate the number of cartons, vials, diluents, and droppers, as per requisition.

3.2 PACKING VACCINES

3.2.1 RESPONSIBILITY

The Storekeeper under the supervision of the Store Officer/Assistant Store Officer is responsible for all packing of vaccines and supplies at the FDI Warehouse.

3.2.2 PROCEDURE

- All the store staff must ensure that they wash their hands thoroughly before handling vaccine cartons and vaccine vials.
- Sort, pick, and pack the different vaccine, as per the packing protocols for each vaccine from the allocated cold/refrigerated rooms.
- Only open the FR/CRs door when necessary; for example, when preparing for vaccine repacking.
- Organize all types of vaccines per the requisition/demand form; segregate them in the different FR/CRs
- For dispatch of vaccines for far destinations and outreach sessions, follow packing protocols for specific vaccines in order to minimize the risk of damaging the vaccines.
- Before packing, prepare conditioned ice packs ([Annex 11](#)) and water coolants, as per the following instructions.

3.2.2.1 Prepare Ice Packs/Cool Water Packs

- Establish requirements: Calculate the number of ice packs/cool water packs/warm water packs needed for each delivery. Calculate how long it will take to prepare them.
- Prepare ice packs: Place the required number of water packs in a freezer room or freezer that is kept at a temperature between -5°C and -25°C. Leave them until they are fully frozen. If an ice pack fast freezer is used to freeze the ice packs, move the fully frozen ice packs to a conventional freezer or to cold boxes for storage purposes.
- Prepare cool water packs: Place the required number of water packs in a cold room or refrigerator that is kept at a temperature between +2°C and +8°C. Leave them to stabilize for a minimum of 12 hours
 - Cold rooms: DO NOT allow the temperature of the cold room to rise above +8°C during the cooling process. DO NOT allow water packs to touch the vaccines.
 - Refrigerators: Use a dedicated refrigerator. DO NOT cool water packs in a refrigerator that contains vaccine.

3.2.3 PACKING PROCEDURES

3.2.3.1 Packing vaccines that are not damaged by freezing

The following vaccines are NOT damaged by freezing. They can safely be packed and transported using fully frozen ice packs at all times of the year.

- ✓ OPV—monovalent, bivalent, and trivalent
- ✓ BCG
- ✓ measles

The following points must be ensured before packing these vaccines:

- Use the correct size and number of ice pack for the chosen cold box. Line the cold box exactly as described on the instructions given inside of the cold box lid.
- Pack the vaccine cartons in the cold box with the vial caps facing up.
- Use newspaper or other loose packing to ensure that the load cannot shift during transport.
- Place a freeze indicator device in the box on top of vaccines.
- Place a packing list in the box on top of the vaccine.

- Label the box with the final destination of placement.
- Close the lid and engage the catch.
- Keep the cold box in the packing room, or in a covered holding area, until all other boxes in the consignment have been packed.
- Keep the cold box away from direct sunlight during transport.

3.2.3.2 Packing freeze-sensitive vaccines using conditioned ice packs

The following vaccines ARE damaged by freezing and must always be packed as described below:

- ✓ hepatitis B (Hep B)
- ✓ pentavalent (DTP-Hep B-Hib)
- ✓ pneumococcal vaccine (PCV-10)
- ✓ tetanus toxoid vaccine (TT)

The following points must be ensured before packing these vaccines:

- Condition the required number of frozen ice packs as described (Annex 14) for conditioning frozen ice packs.
- Use the correct size and number of fully conditioned ice packs for the chosen cold box. Line the cold box exactly as described in the instructions on the inside of the cold box lid.
- Pack the vaccine cartons in the cold box with the vial caps facing up.
- Use newspaper or other loose packing to ensure that the load cannot shift during transport.
- Place a packing list and freeze indicator device in the box on top of the contents.
- Label the box with the final destination of the placement.
- Close the lid and engage the catch.
- Keep the cold box in the packing room, or in a covered holding area, until all other boxes in the consignment have been packed.
- Keep the cold box away from direct sunlight during transport.

3.2.3.3 Packing freeze-sensitive vaccines using cool water packs

The following vaccines ARE sensitive to freezing and must always be packed as described below:

- ✓ hepatitis B (Hep B)
- ✓ pentavalent (DTP-Hep B-Hib)
- ✓ pneumococcal vaccine (PCV-10)
- ✓ tetanus toxoid vaccine (TT)

The following points must be ensured before packing these vaccines:

- Use the correct size and number of cool water packs (+2°C to +8°C) for the chosen cold box. Line the cold box exactly as described in the instructions on the inside of the cold box lid.
- Pack the vaccine cartons in the cold box with the vial caps facing up.
- Use newspaper or other loose packing to ensure that the load cannot shift during transport.
- Place a packing list and freeze indicator device in the box on top of the vaccines.
- Label the box with the final destination of the placement.
- Close the lid and engage the catch.
- Keep the cold box in the packing room, or in a covered holding area, until all other boxes in the consignment have been packed.
- Keep the cold box away from direct sunlight during transport.

3.2.3.4 Packing diluents

- Pack inner diluent cartons in sturdy cardboard boxes or plastic crates.
- Use newspaper or other loose packing to ensure that the load cannot shift during transport.
- Place a packing list in the box on top of the contents.
- Label the carton with the final destination of the placement.
- Keep diluent cartons away from direct sunlight during transport.
- Keep the cold box away from direct sunlight during transport. Repack all the damaged/broken cartons of dry supplies before loading onto the truck.
- Ensure that the cartons are sealed with plastic tape for protection and to ensure the cartons do not break at the edges.

Note: If diluents are frozen, the glass ampoule is likely to break, so they must never be exposed to temperatures below 0°C.

- After packing all the vaccines into cartons, according to set protocols, post tags on each repacked carton that includes the following information, signed by the Storekeeper and Store Officer:
 - ✓ Name of vaccine
 - ✓ Manufacturer
 - ✓ Consignee location to be dispatched
 - ✓ Expiry date of vaccine
 - ✓ Quantity in vials
 - ✓ Number of ice packs
- Provide a packing list/shipment report that includes the following information for all repacked vaccine cartons, duly signed by the Storekeeper and Store Officer
- Ensure that the provided repacking list is used to repack the correct item, and the correct quantity, for the correct stakeholder, and for the correct district.
- Scan the vaccines that have barcodes; update the WMS/vLMIS or stock register.
- For vaccines transported by refrigerated trucks, arrange the truck for the sorted dispatch; load and place the insulated containers of vaccines onto the refrigerated truck.
- Physically count the loaded vaccines in the presence of the truck driver or relevant person who removed the vaccines from the FDI Warehouse.
- The WMS/vLMIS operator generates the electronic issue and dispatch voucher for dispatching the vaccine consignment, which includes the following information, as shown in the figure below:
 - ✓ Reference number of demand letter/requisition
 - ✓ Issue reference
 - ✓ Date/time of issuance
 - ✓ Purpose
 - ✓ Office
 - ✓ Product
 - ✓ Batch number
 - ✓ VVM stage
 - ✓ Quantity in vials
 - ✓ Stock issue voucher in the vLMIS

Stock Issue/Dispatch

Please email support@mis.gov.pk OR contact 011-8180624 Ext. 166 in case of any problem/question.


Fill out this form

Issue No:	Date:	Issue Reference	Purpose *
	23/01/2023 04:37 PM		Stock
Office *			
Select			
Product *	Used for	Manufacturer Batch Quantity Priority *	Location VLM Stage Quantity
Select			NA
Quantity *	Total available batch quantity	Expiry Date	Dispatch By
Unit			

Add Issue

- Prepare and print three copies of the Stock Issue/Dispatch Vouchers from the WMS/vLMIS and get the approval of the relevant authority of the FDI Warehouse.
- The vLMIS operator will issue a gate pass by vLMIS, which has the information for the dispatched quantity to the consignee.
- Give one copy of the issue voucher, signed by the Storekeeper, Store Officer, and receiver, including the gate pass, to the transporter; one copy for the receiver/consignee; and a third copy will be kept at FDI Warehouse as a confirmation that vaccines/supplies were delivered to and received by the consignee.
- Follow up with the freight forwarders/transporter for the timely deliveries of vaccines to the consignee.

The figure below summarizes the process of issuance and dispatch:

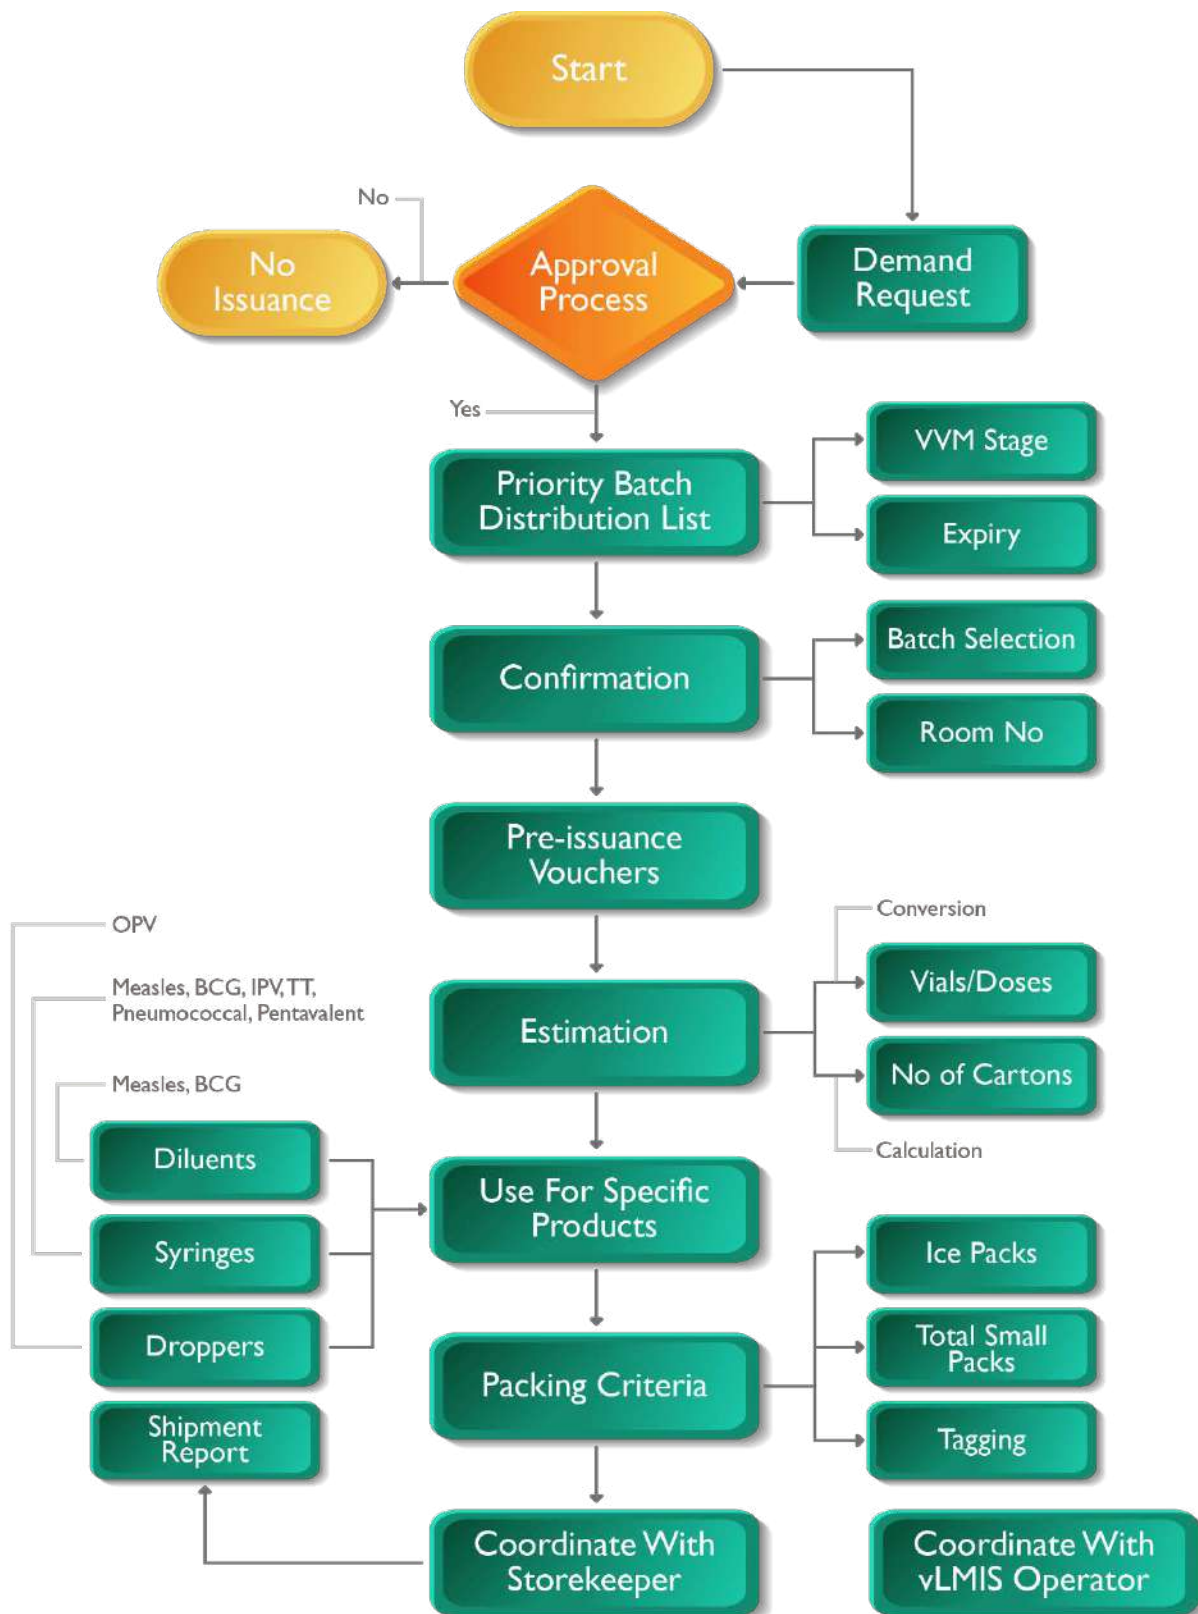


3.3 Reverse Logistics of Pfizer Vaccine

For COVID Pfizer-BioNTech vaccines (Adult and Pediatric), FDI apply Reverse Logistics to return back thermal boxes with Data Loggers to Pfizer for their reuse/recycle purpose as per Pfizer's global contract with donors and governments/countries for vaccine purchase.

Returning thermal shipping containers and real-time temperature monitors to the suppliers will help Pfizer fulfil its commitments to use reusable resources. The following instructions should be taken in accordance with the standard operation procedure to prepare the thermal shipping container for return:

- Upon arrival of Pfizer-BioNTech vaccine boxes at the FDI warehouse, all the Data Loggers to be stopped to secure the data and upload the current data on the Pfizer web portal.
- Properly discard the dry ice. Take necessary precautions by reviewing the Dry Ice Safety Data Sheet.
- Remove the remaining dry ice by leaving it at room temperature in a well-ventilated area. It will change from a solid to a gas. "DO NOT" leave dry ice in an unsecured area.
- Make sure everything to be returned is inside the box, then tape it shut. The return label can be found inside the shipper or already adhered to the inner flap of the thermal shipper.
- Contact the carrier identified on the return label to arrange the return. Followed the Returning Thermal Shipping Container instructions included in the shipper. When coordinating the return of the Soft box thermal shipping container, applied the preprinted return shipping label over the existing shipping label.
- Below diagram illustrate the process of return of thermal shipper soft boxes:

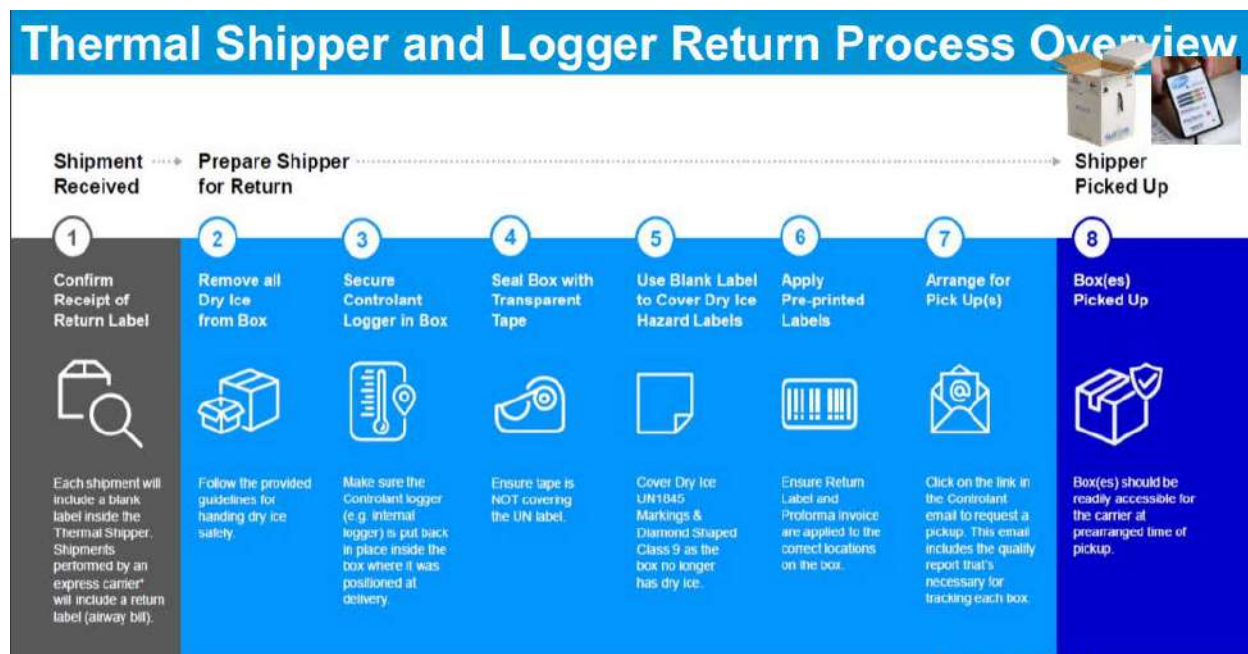

Elements Required for Return

- Thermal Shipping container and inner components
- Temperature Monitoring Device
- Dry Ice Pod

Ensure the Dry Ice UN1845 marking and diamond-shaped Class 9 hazard label on the thermal shipping container are covered by placing a blank label over them in preparation for the return, as the container no longer contains dry ice.

For Soft box, blank sticker labels to place over the UN1845 markings found on the back page of the Shipping and Handling Guidelines.



3.4 DRY STORE

3.4.1 RESPONSIBILITY

The Storekeeper under the supervision of the Store Officer/Assistant Store Officer is responsible for issuing vaccines and supplies to the provinces and districts at the FDI Warehouse.

3.4.2 PROCEDURE

- Acquire the complete signed requisition/demand of compulsory dry supplies from all provinces, including the public and private stakeholders.
- Review and analyze the vaccine supplies requirements for each stakeholder; to fulfill the requirement, check the availability of the dry store stock in the FDI Warehouse.
- Prepare the approval sheet, or the release order request, for the requested supplies for approval from the relevant FDI Warehouse authority.
- The approval sheet should contain the essential information, including the quantity requested by the province and district and the current stock status at the FDI Warehouse.
- The approval sheet for the resale of supplies will include a recommendation to decrease the number of ancillary items of vaccines by the actual demand by clients, upon stock sufficiency analyses.
- Supplies will be issued to all province stakeholders that maintain the minimum/maximum level of vaccine stock at the FDI Warehouse.
- Prepare supplies dispatch order sheet/release order that has all the necessary information related to the requested supplies.
- Follow the criteria of FEFO for dispatch of batches.
- Sort, pick, and pack the different supplies as per the packing protocols of each dry store item, from the allocated racks, pallet location.
- Arrange supplies for loading.
- Arrange the truck for the sorted dispatch; load the consignment of supplies.
- Physically count the loaded supplies in the presence of the truck driver or relevant person who removed supplies from the FDI Warehouse.
- The WMS/vLMIS operator generates the electronic issue and dispatch voucher for dispatching the consignment, which includes the following information, as shown in figure below:
 - ✓ Reference number of demand letter/requisition
 - ✓ Issue reference
 - ✓ Date/time of issuance
 - ✓ Purpose
 - ✓ Office
 - ✓ Product
 - ✓ Batch number
 - ✓ Quantity in vials.

Stock Issue/Dispatch

Please email support@mis.gov.pk OR contact 011-9380024 Ext. 166 in case of any problem/question.

Fill out this form

Issue No:	Date:	Issue Reference	Purpose *
	23/01/2023 04:37 PM		Stock
Office *			
Product *	Used for	Manufacturer Batch Quantity Priority *	Location VLM Stage Quantity
			NA
Quantity *	Total available batch quantity	Expiry Date	Dispatch By
Unit			

Add Issue

- Prepare and print three copies of the Issue/Dispatch vouchers from the WMS/vLMIS and get the approval of the relevant authority of the FDI Warehouse.
- The vLMIS operator will issue a gate pass by vLMIS, which has the information of the dispatched quantity to the consignee.
- Give one copy of the Issue/Dispatch voucher signed by the Storekeeper, Store Officer, and receiver, and including the Gate Pass to the transporter; one copy for the receiver/consignee; and a third copy will be kept at the FDI Warehouse as a confirmation that supplies were delivered to and received by the consignee.
- Follow up with the freight forwarders/transporter for the timely delivery of supplies to the consignee.

4.0 DISPOSAL

4.1 UNUSABLE VACCINE

4.1.1 RESPONSIBILITY

The Storekeeper under the supervision of the Store Officer/Assistant Store Officer is responsible for the maintenance and disposal of unusable vaccines and supplies.

4.1.2 PROCEDURE

- If, for any reason, vaccines are identified as unusable (expired, physically damaged from heat exposure and freezing etc.), the relevant FDI Warehouse or store authority should immediately stop distributing the unusable vaccine stock.
- Immediately separate the identified vaccine lot, batch, or any quantity identified in the FDI Warehouse as unusable stock.
- Store the container having unusable vaccines in a cold room or vaccine refrigerator until permission is given to take it out of the cold chain.
- Clearly mark the assigned storage area as “EXPIRED VACCINES FOR DISPOSAL-DO NOT USE,” in the case of expired vaccines.
- Clearly mark as “DAMAGED VACCINES FOR DISPOSAL-DO NOT USE” in case of physically damaged vaccines, due to heat exposure (VVM color change) and freezing, so that items placed here cannot be confused with usable stock.
- If diluents also need to be removed from stock, place them in a container clearly marked “EXPIRED DILUENTS FOR DISPOSAL—DO NOT USE.”
- Record and update the vLMIS regarding the expired vaccines or diluents. Prepare a loss and adjustment report.
- Immediately notify the relevant FDI Warehouse or store office authorities through the proper procedures and policies of the FDI Warehouse.
- By providing a detailed description of the unusable vaccine, the relevant FDI Warehouse higher authority can initiate further actions and can form a committee to identify why the vaccine stock was found unusable and arrange for its safe disposal.
- The committee will advise the FDI Warehouse relevant authority how to safely dispose of the unusable vaccines and diluents.
- The committee may finally decide to dispose of or use the identified vaccine stock, based on laboratory tests and other findings from the vaccine stock inspection.
- Hazardous/infectious vaccine waste must be disinfected and buried, incinerated, or disposed of by following specific and established procedures for disposing of vaccines ([Please refer the FDI Logistics Manual](#)).
- To ensure that expiries or damages do not occur again, the committee will provide a detailed report on the expiries or damaged vaccines stock, and the action and corrections that took place.

4.2 DAMAGED ANCILLARY ITEMS

- If, for any reason, ancillary items are identified as unusable (expired, damaged, etc.), the relevant FDI Warehouse or store authority should immediately stop distribution of the unusable stock.
- Immediately separate the identified lot, batch, or any quantity identified in the FDI Warehouse as unusable stock.
- Assign a separate well-ventilated room for these products. Clearly mark the assigned storage “PRODUCTS FOR DISPOSAL—DO NOT USE” so that items placed here cannot be confused with usable stock.
- Immediately notify the relevant FDI Warehouse or store authority through the proper procedures and policies of the FDI Warehouse.
- By providing a detailed description of the unusable ancillary items, the relevant FDI Warehouse higher authority can initiate further actions and can form a committee to identify why the stock was damaged or expired and arrange for its safe disposal.
- The committee will advise the FDI Warehouse relevant authority how to safely dispose of the unusable supplies.
- The committee may finally decide to dispose of the unusable stock either through incineration or by landfill. Other methods may include inertization, chemical treatment, or by using sharps pits.
- To ensure that expiries or damages do not occur again, the committee will provide a detailed report on the expiries or damaged vaccines stock, and the action and corrections that took place.

5.0 ANNEXURES

COLD STORE

ANNEX-1 SHIPPING INFORMATION (SAMPLE)

scan
GLOBAL LOGISTICS

****PRE-ADVICE****

To: UNICEF PAKISTAN
From: CJ KOREA EXPRESS
Pages: Total 09 pages including Pre-Advice Cover Sheet
Date: 2016. 02. 02
Re.: 45143062 - 6 PART SIX

PO NUMBER: 45143062
CUST. REF.: PSS-GAVI-PAK-15 PENTA VA
PCS: 93
KGS: 4,557KG
CBM: 29.40CBM
COMMODITY: DTP-HepB-Hib fully liquid vaccine
NUMBER OF VIALS: 390,000
VALUE: USD916,500.00
AWB NO.: 157-9437 8760

FLIGHT: ICN / DOH QR859/17.FEB (00:05-04:15)
DOH/ISB QR632/17.FEB (19:40-01:00)+1

ETA ISB : 01:00 HRS / 18 FEB 2016

Yours sincerely
Scan Global Logistics A/S

국립중앙의료원/국립중앙의료원/20160202/133716

Crucell

Berna Biotech Korea Corp.

Summary Protocol for the Production and Testing of DTwP-HepB-Hib Fully Liquid Combination Vaccine

FINAL PRODUCT

IDENTIFICATION OF FINAL LOT

Name and address of manufacturer	Berna Biotech Korea Corp. (Seongdo-dong) 23, Harmony-ro 303beon-gil, Yeosu-su-gu, Incheon, 406-840 Korea
International name and proprietary name of vaccine	Diphtheria-Tetanus-Whole Cell Pertussis-Hepatitis B (cDNA)- <i>Histophilus influenzae</i> type b-conjugated to Diphtheria CRM197 Combination Vaccine (DTwP-HepB- Hib Fully Liquid Combination Vaccine), Quinvaxem® inj.
Lot number of final product	1453338
Date of manufacture of final lot	2014.08.25.
Type of container	Vial
Quantity of manufacture (unit : vials)	726,432
Number of doses in each container	1 dose/vial
Volume of single dose	0.5 mL/dose
Expiry date	2017.08.24.

Quinvaxem® inj.	Berna Biotech Korea Corp.	Lot No. 1453338
Summary Protocol (Ver. 2.1)		Page 1 of 16

29

Remet à l'adresse de l'Expéditeur Shipper's Name and Address SANOFI PASTEUR C/O UNICEF SUPPLY DIVISION OCEANJEV 10-12 DK-2100 COPENHAGEN		Numéro de compte de l'Expéditeur Shipper's Account Number FEDERAL EXPANDED PROGRAMME ON IMMUNIZATION, MINISTRY OF NATIONAL HEALT SERVICE REGULATIONS AND COORDINATION CHAK SHAHZAD, ISLAMABAD, PAKISTAN		LETTRE DE TRANSPORT EMIRATES AERIEN Non négociable PO BOX 666 Service par DUBAI Non négociable AE UNITED ARAB EMIRATES Issued by Les exemplaires 1, 2 et 3 de cette lettre de transport aérien sont originaux et ont la même validité Copies 1, 2 and 3 of this Air Waybill are originals and have the same validity.	
Nom et adresse de destination Consignee's Name and Address FEDERAL EXPANDED PROGRAMME ON IMMUNIZATION, MINISTRY OF NATIONAL HEALT SERVICE REGULATIONS AND COORDINATION CHAK SHAHZAD, ISLAMABAD, PAKISTAN		Numéro de compte du destinataire Consignee's Account Number R est convenu que les marchandises (autres que les précieuses) sont acceptées pour le transport sur base d'un accord tacite souscrit par le transporteur et le destinataire. Les marchandises peuvent être transportées par tout autre moyen et sous réserve de l'avis de l'expéditeur. Les marchandises peuvent être transportées par tout autre moyen et sous réserve de l'avis de l'expéditeur. Les marchandises peuvent être transportées par tout autre moyen et sous réserve de l'avis de l'expéditeur.		R est convenu que les marchandises (autres que les précieuses) sont acceptées pour le transport sur base d'un accord tacite souscrit par le transporteur et le destinataire. Les marchandises peuvent être transportées par tout autre moyen et sous réserve de l'avis de l'expéditeur. Les marchandises peuvent être transportées par tout autre moyen et sous réserve de l'avis de l'expéditeur. Les marchandises peuvent être transportées par tout autre moyen et sous réserve de l'avis de l'expéditeur.	
Nom et ville de l'agent de l'expéditeur Issuing Office's Name and City ND OVERSEAS FRANCE RUE DU CHAPELIER ZONE DE FRET 4 AEROPORT ROISSY CDG		Nom et ville de l'agent du destinataire Issuing Office's Name and City ND OVERSEAS FRANCE RUE DU CHAPELIER ZONE DE FRET 4 AEROPORT ROISSY CDG		Références complètes Accounting Information *** SEX *** SEX *** SEX *** EXPEDITION APTE AU TRANSPORT AERIEN MRN AGENT HABILITE FR/RA/04018-01/0000	
Code AEA de l'agent de l'expéditeur Issuing Office's AEA Code 2047978/9512		Code AEA de l'agent du destinataire Issuing Office's AEA Code 2047978/9512		N° de Référence Reference Number FR/RA/04018-01/0000	
Adresse de départ (adresse de l'expéditeur) Address of Origin (Address of Shipper) ROISSY CDG		Adresse de destination (adresse du destinataire) Address of Destination (Address of Consignee) ROISSY CDG		Informations relatives au transport Shipping Information ROISSY CDG	
À l'ordre de For order of DKX		À l'ordre de For order of DKX		À l'ordre de For order of DKX	
À l'ordre de For order of DKX		À l'ordre de For order of DKX		À l'ordre de For order of DKX	
À l'ordre de For order of DKX		À l'ordre de For order of DKX		À l'ordre de For order of DKX	
À l'ordre de For order of DKX		À l'ordre de For order of DKX		À l'ordre de For order of DKX	
À l'ordre de For order of DKX		À l'ordre de For order of DKX		À l'ordre de For order of DKX	
À l'ordre de For order of DKX		À l'ordre de For order of DKX		À l'ordre de For order of DKX	
À l'ordre de For order of DKX		À l'ordre de For order of DKX		À l'ordre de For order of DKX	
À l'ordre de For order of DKX		À l'ordre de For order of DKX		À l'ordre de For order of DKX	
À l'ordre de For order of DKX		À l'ordre de For order of DKX		À l'ordre de For order of DKX	
À l'ordre de For order of DKX		À l'ordre de For order of DKX		À l'ordre de For order of DKX	
À l'ordre de For order of DKX		À l'ordre de For order of DKX		À l'ordre de For order of DKX	
À l'ordre de For order of DKX		À l'ordre de For order of DKX		À l'ordre de For order of DKX	
À l'ordre de For order of DKX		À l'ordre de For order of DKX		À l'ordre de For order of DKX	
À l'ordre de For order of DKX		À l'ordre de For order of DKX		À l'ordre de For order of DKX	
À l'ordre de For order of DKX		À l'ordre de For order of DKX		À l'ordre de For order of DKX	
À l'ordre de For order of DKX		À l'ordre de For order of DKX		À l'ordre de For order of DKX	
À l'ordre de For order of DKX		À l'ordre de For order of DKX		À l'ordre de For order of DKX	
À l'ordre de For order of DKX		À l'ordre de For order of DKX		À l'ordre de For order of DKX	
À l'ordre de For order of DKX		À l'ordre de For order of DKX		À l'ordre de For order of DKX	
À l'ordre de For order of DKX		À l'ordre de For order of DKX		À l'ordre de For order of DKX	
À l'ordre de For order of DKX		À l'ordre de For order of DKX		À l'ordre de For order of DKX	
À l'ordre de For order of DKX		À l'ordre de For order of DKX		À l'ordre de For order of DKX	
À l'ordre de For order of DKX		À l'ordre de For order of DKX		À l'ordre de For order of DKX	
À l'ordre de For order of DKX		À l'ordre de For order of DKX			

ANNEX 3- PACKING LIST (SAMPLE)

PACKING LIST 24.08.2015 Page 1/1					SANOPI PASTEUR 	
DELIVERY NR : 0080591591					ORDER NR : 0000164340	
CONSIGNER sanofi pasteur 2 Avenue Pont Pasteur Boite Postale : BP 7046 69367 LYON Cedex 07 France					CONSIGNEE FEDERAL EXPANDED PROGRAMME ON IMMUNIZATION, MINISTRY OF NATIONAL HEALTH SERVICE REGULATIONS AND COORDINATION CHAK SHAHZAD / ISLAMABAD Pakistan	

NR PACKAG E	GROSS WGHT BY PACKAGE	NET WEIGHT BY PACKAGE	VOLUME BY PACKAGE	LxHxW		
	MATERIAL DESCRIPTION			BATCH NR	SHELF LIFE	QUANTITY BY PACKAGE
1 to 19	53,640	37,312	0,215	71X60,8X50		
	456 BOPV1+3 10F 20D VVM XFAE PU			L5445-1	30.09.2016	440
20	49,740	33,072	0,215	71X60,8X50		
	456 BOPV1+3 10F 20D VVM XFAE PU			L5445-1	30.09.2016	390
21 to 37	9,004	7,500	0,089	51X39X45		
	COMPTE-GOUTTE 13MM NON STERILE			14J134	01.10.2019	500
38	5,070	3,750	0,071	46X43,5X35,5		
	COMPTE-GOUTTE 13MM NON STERILE			14J134	01.10.2019	250

NUMBER OF PACKAGES:	38
TOTAL GROSS WEIGHT (KG)	1227,040
TOTAL NET WEIGHT (KG)	873,250
TOTAL VOLUME (M3) :	5,884

ANNEX 4- INVOICE (SAMPLE)

SANOFI PASTEUR Siège mondial : 2, avenue Pasteur - F-69367 Lyon cedex 07 Tél. : +33 (0)4 37 37 01 00 - Fax : +33 (0)4 37 37 78 30 N° ID TVA FR 54 349 505 370		SANOFI PASTEUR	
24.08.15	INVOICE ORIGINAL	90106418 164340	1 101446 PO 45141516
FEDERAL EXPANDED PROGRAMME ON IMMUNIZATION, MINISTRY OF NATIONAL HEALTH SERVICE REGULATIONS AND COORDINATION CHAK SHAHZAD / ISLAMABAD Pakistan		UNICEF Supply Division Oceanvej 10-12 2100 COPENHAGEN Denmark 45/35273527 Id. VAT : DK34529809	
DATE	31.08.15	ND-OVERSEAS France	ND-OVERSEAS France
QUANTITY	38	1.227,040	873,250
PRICE	5,884		
CONDITION OF STORAGE / Stockage : -20°C			
QUANTITY	8.750	28,00000	245.000,00
PRICE	8.750		
QUANTITY	8.750	8.750	
PRICE	8.750		
EXONERATED TRANSACTION FOR EXPORTATION VAT treatment: tax exempt export according to paragraph 1 of article 146 of directive 2006/112/EC Supplier reference: LTA 42104385 Unicef Reference: 10015812 PAK			
QUANTITY	245.000,00	USD	245.000,00
PRICE	USD		
BANK TRANSFER 30 DAYS END MONTH AFTER SHIPME 30.09.2015			
NATIXIS 19, PL TOLOZAN			
101446 24.08.2015			

ANNEX 5- RELEASE CERTIFICATE (SAMPLE)



Country	:Pakistan
Customer	:100426, UNICEF
Order	:7100016501/000020

CERTIFICATE OF RELEASE

Manufacturer	GlaxoSmithKline Biologicals Rixensart - Belgium
Product	Synflorix
Product description	Streptococcus Pneumoniae Polysaccharide Serotype (1,5,6B,7F,9V,14,23F) -PD Conjugate (1µg/d), Serotype 4-PD Conjugate (3µg/d), Serotype 18C-TT-AH Conjugate (3µg/d), Serotype 19F-DT Conjugate (3µg/d) Vaccine
Batch number	ASPNA754BA
Quantity	167.100 X 2 dose(s)
Expiry	November/2017
Date of manufacture	December/2014

I hereby confirm that this batch has been manufactured and controlled in compliance with the cGMP regulations and in accordance with the local regulatory requirements of the receiving market . This includes that, for any materials derived from ruminants (bovine, ovine, caprine) used in the manufacture and/or formulation of the batch of product specified above, all measures have been taken to demonstrate compliance with Directive 2001/83/EC and amending Directives 2003/63/EC and 2004/27/EC

Sarah LOUAGIE
Industrial Pharmacist

15 JUL. 2015



p.o. Eric Sarlet
Qualified Person
QA Director
GSK Biologicals
Rue de l'Institut 89
1330 Rixensart
Belgium

ANNEX 6- PROTOCOL CERTIFICATE (SAMPLE)

NL41008

BRP Version: 1.0


Document Name	Document Number	BRP Version Number
BRP - L5444 - STD (09-Apr-2015) - 1.0	BRP_327408	1.0
RELEASE PROTOCOL - BIVALENT ORAL POLIOMYELITIS VACCINE - Lot L5444		

	Approver Name	Date (Universal Time)	Reason for Signature
Approval	VERNEZ Stéphane	09 Apr 2015 17:01:13	I am approving this document
	Effective Date:	09 Apr 2015	

Electronically approved by Qualified Person : The above electronic signature is legally binding and equivalent to individual's hand written signature as per the GMP and 21 CFR Part 11.

ANNEX 7- VACCINE ARRIVAL REPORT (SAMPLE)

This VAR is designed for any comments about the shipment, for example:

VACCINE ARRIVAL REPORT (VAR) ¹																																																																																																											
This report is to be filled in by authorized staff, ratified by the Store Manager or the EPI Manager, and forwarded to the procurement agency within three days of vaccine arrival. Use one report for each vaccine in the shipment.																																																																																																											
COUNTRY		REPORT No.		Date of report																																																																																																							
Place, date and time of inspection				Name of cold store, date and time vaccines entered into cold store																																																																																																							
PART I — ADVANCE NOTICE																																																																																																											
MAIN DOCUMENTS		Date received by consignee		Copy airway bill (AWB)		Copy of packing list		Copy of invoice		Copy of release certificate																																																																																																	
Pre-advance																																																																																																											
Shipping notification		Yes ☐ No ☐		Yes ☐ No ☐		Yes ☐ No ☐		Yes ☐ No ☐		Yes ☐ No ☐																																																																																																	
List other documents (if requested)																																																																																																											
PART II — FLIGHT ARRIVAL DETAILS																																																																																																											
AWB Number		Airport of destination		Flight No		ETA as per notification		Actual time of arrival																																																																																																			
						Date		Time		Date																																																																																																	
NAME OF CLEARING AGENT: _____ ON BEHALF OF: _____																																																																																																											
PART III — DETAILS OF VACCINE SHIPMENT																																																																																																											
Purchase Order No.		Consignee		Vaccine description (Type and doses/vial)				Manufacturer		Country																																																																																																	
<table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th colspan="4" style="text-align: center;">Vaccine</th> <th colspan="4" style="text-align: center;">Diluent/droppers</th> </tr> <tr> <th>Lot Number</th> <th>Number of boxes</th> <th>Number of vials</th> <th>Expiry date</th> <th>Lot Number</th> <th>Number of boxes</th> <th>Number of units</th> <th>Expiry date</th> </tr> </thead> <tbody> <tr><td> </td><td> </td><td> </td><td> </td><td> </td><td> </td><td> </td><td> </td></tr> <tr><td> </td><td> </td><td> </td><td> </td><td> </td><td> </td><td> </td><td> </td></tr> <tr><td> </td><td> </td><td> </td><td> </td><td> </td><td> </td><td> </td><td> </td></tr> <tr><td> </td><td> </td><td> </td><td> </td><td> </td><td> </td><td> </td><td> </td></tr> <tr><td> </td><td> </td><td> </td><td> </td><td> </td><td> </td><td> </td><td> </td></tr> <tr><td> </td><td> </td><td> </td><td> </td><td> </td><td> </td><td> </td><td> </td></tr> <tr><td> </td><td> </td><td> </td><td> </td><td> </td><td> </td><td> </td><td> </td></tr> <tr><td> </td><td> </td><td> </td><td> </td><td> </td><td> </td><td> </td><td> </td></tr> <tr><td> </td><td> </td><td> </td><td> </td><td> </td><td> </td><td> </td><td> </td></tr> <tr><td> </td><td> </td><td> </td><td> </td><td> </td><td> </td><td> </td><td> </td></tr> </tbody> </table>												Vaccine				Diluent/droppers				Lot Number	Number of boxes	Number of vials	Expiry date	Lot Number	Number of boxes	Number of units	Expiry date																																																																																
Vaccine				Diluent/droppers																																																																																																							
Lot Number	Number of boxes	Number of vials	Expiry date	Lot Number	Number of boxes	Number of units	Expiry date																																																																																																				
(Continue on separate sheet if necessary)																																																																																																											
<table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th></th> <th>Yes</th> <th>No</th> <th>Comments</th> </tr> </thead> <tbody> <tr> <td>Was quantity received as per shipping notification?</td> <td>☐</td> <td>☐</td> <td> </td> </tr> <tr> <td>If not, were details of short-shipment provided prior to vaccine arrival?</td> <td>☐</td> <td>☐</td> <td> </td> </tr> </tbody> </table>													Yes	No	Comments	Was quantity received as per shipping notification?	☐	☐		If not, were details of short-shipment provided prior to vaccine arrival?	☐	☐																																																																																					
	Yes	No	Comments																																																																																																								
Was quantity received as per shipping notification?	☐	☐																																																																																																									
If not, were details of short-shipment provided prior to vaccine arrival?	☐	☐																																																																																																									
¹ Adopted from the Standard UNICEF Vaccine Arrival Report from WHO Guidelines on the international packaging and shipping of vaccines (WHO/VB05.23) No. = Number WHO recommends all UN agencies, countries and non-governmental organizations procuring vaccines adopt this report.																																																																																																											

Page 2

- condition of the shipping cartons, inner boxes, vials, and droppers
- labeling on the shipping cartons—this should include a warning regarding the temperature-sensitive nature of vaccines and the shipment details (purchase order number, consignee information, and shipping carton number)
- labeling on the inner boxes and vials
- observations on any stages of the vaccine vial monitors (VVM)
- general condition of the shipment
- comments related to any previous sections of the VAR, such as documentation, delays, short shipment, or shipping indicators

ANNEX 8 – USING THE VACCINE VIAL MONITOR

A1.1: What is a VVM?

A VVM is a heat-sensitive label that is placed on a vaccine vial to register cumulative heat exposure, over time. The VVM is a circle with a small square inside it. The square contains a heat-sensitive dye.

A1.2: How does it work?

The combined effects of time and temperature cause the inner square of the VVM to darken—gradually and irreversibly:

- The lower the temperature, the slower the inner square changes color
- The higher the temperature, the faster the inner square changes color

A1.3: What are its limitations?

The VVM does not directly measure vaccine potency, but it does give information about the main factor that affects potency: heat exposure over a period of time.

Many liquid vaccines are also damaged by exposure to freezing. The VVM does **not** register information about freezing.

A1.4: What are the VVM stages?

There are only two WM stages:

- The **usable** stage is when the square is lighter than the circle
- The **unusable** stage is when the square matches the color of the circle, or is darker
- The **end point** is when the color of the square exactly matches the color of the circle

A1.5: How to read a VVM

Unusable stage

The square is lighter than the circle. If the square matches the color of the circle or is darker if the expiry date is not passed, the circle.

A1.6: Why are VVMs important?

The VVM shows whether the vaccine vial has been exposed to excessive heat, over time, and it indicates whether the vaccine is likely to have been damaged by this exposure. After the indicator reaches the **end point**, the vaccine should not be used.

A1.7: What types of VVM are available and how are they used?

Some vaccines are more sensitive to heat than others. For this reason, currently, four different types of VVMs are designed to match vaccines with differing heat stability. For example, VVM 2 is used with OPV because this is the most heat-sensitive vaccine; this VVM reaches its discard point after only 2 days at 37°C. In contrast,

hepatitis B vaccine is very heat-stable and the VVM 30 is used; it takes 30 days to reach its discard point at 37°C.

The table below describes the four VVM reaction rates by category of heat stability.

VVM Reaction Rates by Category of Heat Stability

Category		Time to End Point at +37°C	Time to End Point at +25°C	Time to End Point at +5°C
VVM 30 High stability		30 days	193 days	>4 years
VVM 14 Medium stability		14 days	90 days	>3 years
VVM 7 Moderate stability		7 days	45 days	>2 years
VVM 2 Least stable		2 days	Not applicable	225 days

Note that vaccines made by different manufacturers can have different heat stability characteristics; the World Health Organization (WHO) will assign the different VVM categories. For example, one manufacturer's BCG might use VVM 30, while another type of BCG may need a VVM 14.

A1.8: Where is the VVM located?

VVMs are fixed to the vial or ampoule label of liquid vaccines. Under the Multi-dose Vial Policy (MDVP), they can be used in subsequent sessions. When the vaccine cannot be used in subsequent sessions—for example, lyophilized vaccines, such as measles, mumps, rubella (MMR)—the VVM is fixed to the vial cap or the neck of the ampoule. The VVM can also be fixed to the cap of the mono-dose vials.

Checking the VVM:

- VVM status should be checked at the following times:
 - VVM status should be checked when vaccines are received at the FDI Warehouse.
 - When vaccines are issued by a store.
 - Check VVM status and expiry dates for each type and batch of vaccine when preparing the issued voucher. Generally, make sure that any vaccine that shows the most VVM exposure is issued first.
 - Immediately before opening the vial, check that the VVM status is usable and check that the expiry date has not passed. If both these checks are OK, use the vaccine.
 - If the VVM status is unusable OR the expiry date has passed, **do not** use the vaccine.
 - Put the vaccine to one side until the end of the session and then safely dispose of it.

ANNEX 9- SHAKE TEST PROTOCOL

Vaccine Shake Test

The Shake Test is designed to determine whether aluminum-adsorbed vaccines have been frozen. Whenever it is suspected that vaccine has been frozen, at least one member of the duty personnel in every facility that stores vaccines should know how to perform and interpret the test reliably and correctly. Vaccine that fails the Shake Test should not be distributed or administered.

This annexure explains when to do the Shake Test and what to do if the vaccine has been damaged by freezing. The Shake Test protocol is attached as annex 2; there is only one correct way to conduct this test.

Applicability

The Shake Test currently applies to the following vaccines:

- pentavalent
- pneumococcal
- tetanus toxoid

After freezing, the bonds between the aluminum adsorbent and the antigen in a vaccine are broken. Separated adsorbent tends to form larger, heavier granules that gradually settle at the bottom of the vial when it is shaken. Sedimentation occurs faster in a vaccine vial that has been frozen than in a vaccine vial from the same manufacturer that has never been frozen.

When carried out correctly the Shake Test has been shown to have 100% sensitivity and 100% specificity and 100% positive predictive value.

When and How to Do a Shake Test

If a freeze indicator, or other temperature monitoring device, shows a freeze alarm, or if Store Keeper suspects that freezing has occurred, then the Shake Test must be done to confirm the status of the vaccine. Follow the Shake Test protocol exactly as described in *annex 2*.

Individual batches of vaccine may behave differently from one another. Therefore, the procedure should be repeated with **all** suspect batches.

The Shake Test does **not** need to be conducted under the following circumstances:

- When vaccine vial(s) are frozen solid
- With pentavalent vial(s), after vigorous shaking, it is **impossible** to obtain a homogeneous solution. In such cases, the white lumps or sediment cannot be separated from the walls of the glass vial. This only happens with pentavalent vials if they have been exposed to sub-zero temperatures, but they did not freeze

NOTES:

1. There is only one correct way to conduct a Shake Test.
2. The test procedure described below should be repeated with all suspect batches. In the case of international arrivals, the Shake Test should be conducted on a random sample of vaccines. However, if more than one lot is in the shipment, the random sample must include a vial taken from each and every lot.

NOTES:

1) This protocol must not be altered. There is only one correct way to conduct a Shake Test.	
2) The test procedure described below should be repeated with all suspect batches. In the case of international arrivals, the Shake Test should be conducted on a random sample of vaccine. However, if there is more than one lot in the shipment, the random sample must include a vial taken from each and every lot.	
1. Take a vial of vaccine of the same type and batch number and made by the same manufacturer as the vaccine you want to test.	
2. Clearly mark the vial as “FROZEN.”	
3. Freeze the vial in a freezer, or the freezing compartment of a refrigerator, until the contents are completely solid.	
4. Let it thaw. Do NOT heat it!	
5. Take your “TEST” vial from the batch that you suspect has been frozen.	
6. Hold the “FROZEN” vial and the “TEST” vial together in one hand.	
7. Shake both vials vigorously for 10–15 seconds.	
8. Place both vials on a flat surface side-by-side and start continuous observation of the vials until test is finished. <i>(NOTE: If the vials have large labels that conceal the vial contents, turn both vials upside down and observe sedimentation in the neck of the vial.)</i>	
Use an adequate source of light to compare the sedimentation rates between vials. IF—	
9. The TEST vial sediments slower than the FROZEN vial, THEN,	10. Sedimentation is similar in both vials OR The TEST vial sediments faster than the FROZEN vial THEN,
11. Use the vaccine batch.	11. <u>Vaccine is damaged:</u> Notify your supervisor. Set aside all affected vaccine in a container marked “DAMAGED VACCINE FOR DISPOSAL– DO NOT USE.”
	12. Discard all affected vaccine after you receive permission to do so.
	13. Fill in the Loss/Adjustment Form.

ANNEX 10- ELECTRONIC DEVICE REPORT FORM (SAMPLE)

Reporting ALARM details in international vaccine shipments

A special form has been designed for the purpose of reporting alarm details displayed in electronic devices. This form should ONLY be filled in if any alarms have occurred and should be attached to the Vaccine Arrival Report (VAR). A clear photocopy and/or printed copy of the scanned image of the electronic devices displaying alarm status should be attached to this form.

ELECTRONIC DEVICE ALARM REPORT FORM

Country				Date of receipt			
Type of Device				Type of Vaccine			
Q-Tag 2Plus Syntemp II OMS							

Box	Serial	Time	Elapsed transit time	≥45°C 1		≥30°C 10 hrs		≥10°C 20		≤-0.5°C 1	
				Time	°C	Time	°C	Time	°C	Time	°C

ANNEX 11-CONDITIONING FROZEN ICE PACKS

A3.1: What is a conditioned ice pack?

When an ice pack is removed from the ice pack freezer, its temperature may be as low as -20°C . If you use these ice packs immediately, there is a risk that you will damage freeze-sensitive vaccines.

A *conditioned* ice pack is an ice pack that has been left outside the freezer for long enough to stabilize at 0°C . This point is reached when the ice inside the ice pack begins to melt.

A3.2: How do I know when an ice pack is conditioned?

An ice pack is conditioned as soon as the ice core inside the pack is surrounded by a small amount of liquid water. You can check this by shaking the ice pack. If you can feel the ice moving inside the pack, it is fully conditioned. This process takes time—up to 30 minutes or more, depending on the temperature of the room.

A3.3: When should conditioned ice packs be used?

Conditioned ice packs must ALWAYS be used whenever you pack the following freeze-sensitive vaccines in a cold box or vaccine carrier:

- pentavalent
- PCV-10
- tetanus toxoid

You must also use conditioned ice packs whenever you pack a load of vaccines that contain freeze-sensitive products mixed together with—

- BCG
- OPV
- measles


You DO NOT need to use conditioned ice packs when you pack only OPVs.

A3.4: How to condition ice packs

1. Calculate how many ice packs are needed for the vaccine consignment. The underside of the lid of the cold box or vaccine carrier usually has a diagram showing the number required for that type of box or carrier.
2. Remove the correct number of ice packs from the freezer.
3. Lay the ice packs on the designated table or works surface in a single layer leaving a 5 cm space around each pack.
4. Check their progress every 10 minutes by shaking a sample of ice packs, as shown below.
5. Wait until ALL the ice packs are conditioned; then use them to line the cold boxes and/or vaccine carriers. Pack the vaccine.

DRY STORE

ANNEX 12- PACKING LIST (SAMPLE)



admo
Abu Dhabi Commercial Company

Packing List

Consignment: X330/02

FEDERAL EXPANDED PROGRAMME ON IMMUNIZATION
MONHSRC (MINISTRY OF NATIONAL HEALTH SERVICES REGULATION AND COORDINATION)
CHAK SHAHZAD
ISLAMABAD
PAKISTAN
 Phone: (92) 51 9255101
 Fax: (92) 51 9255086

Purchase Order Number: 45139132
INVOICE Material Number: S0782153
Country of Destination: Pakistan via Karachi
Invoice Reference No.: AD669-05/2015
Date: 30.05.2015
Sales Order No.: 310000896

Item No	Description of Contents	Carton Number	Total No. of Cartons	Quantity per Carton 1,300 Pcs	Gross Weight (Kg)	Dimensions Per Carton / mm	Cubic Measurement (CBM)	Batch / Lot No.	MFG. Date	Expiry Date	
00010	Syringes, auto-disable, 0.5ml with needle and protective cap, blister packed box of 100, 0.5ml syringe with fix needle 23G x 1" (0.6mm x 25mm) and protective cap, auto-disable, blister packed Pre-set volume limit with a graduated scale on the barrel, easy to read Graduation, two markings, 0 and 0.5ml Brand "MEDECO Inject"	40' HC Container:									
		1	77	77	100,100	436.9	844 x 162 x 408	4.30	8915/08	May 2015	Apr 2020
		78	257	180	234,000	1,026.0	844 x 162 x 408	10.04	9015/14	Apr 2015	Mar 2020
		258	531	274	356,200	1,561.8	844 x 162 x 408	15.29	9015/15	Apr 2015	Mar 2020
		532	805	274	356,200	1,561.8	844 x 162 x 408	15.29	9015/16	Apr 2015	Mar 2020
		808	1079	274	356,200	1,561.8	844 x 162 x 408	15.29	9015/17	Apr 2015	Mar 2020
		1080	1175	96	124,600	547.2	844 x 162 x 408	5.36	9015/18	Apr 2015	Mar 2020
		Sub Total:									
		1,178	1,178	1,527,500	2,832	844 x 162 x 408	35.37				
		40' HC Container:									
		1178	1353	178	231,400	1,014.6	844 x 162 x 408	9.93	9015/19	Apr 2015	Mar 2020
		1354	1610	163	211,900	929.1	844 x 162 x 408	9.10	9015/19	Apr 2015	Mar 2020
		1611	1700	274	356,200	1,561.8	844 x 162 x 408	15.29	9015/20	Apr 2015	Mar 2020
		1791	2064	274	356,200	1,561.8	844 x 162 x 408	15.29	9015/21	Apr 2015	Mar 2020
		2065	2338	274	356,200	1,561.8	844 x 162 x 408	15.29	9015/22	Apr 2015	Mar 2020
		2339	2350	12	15,600	68.4	844 x 162 x 408	0.67	9015/23	Apr 2015	Mar 2020
		Sub Total:									
		1,178	1,178	1,527,500	2,832	844 x 162 x 408	35.37				
		40' HC Container:									
		2351	2512	292	340,600	1,493.4	844 x 162 x 408	14.62	9015/23	Apr 2015	Mar 2020
		2513	2880	274	356,200	1,561.8	844 x 162 x 408	15.29	9015/24	Apr 2015	Mar 2020
		2887	3160	274	356,200	1,561.8	844 x 162 x 408	15.29	9015/25	Apr 2015	Mar 2020
		3161	3434	274	356,200	1,561.8	844 x 162 x 408	15.29	9015/26	Apr 2015	Mar 2020
		3435	3525	91	118,300	518.7	844 x 162 x 408	5.08	9015/27	Apr 2015	Mar 2020
		Sub Total:									
		1,178	1,178	1,527,500	2,832	844 x 162 x 408	35.37				
		40' HC Container:									
		3526	3708	183	237,900	1,043.1	844 x 162 x 408	10.21	9015/27	Apr 2015	Mar 2020
		3709	3982	274	356,200	1,561.8	844 x 162 x 408	15.29	9015/28	Apr 2015	Mar 2020
		3983	4256	274	356,200	1,561.8	844 x 162 x 408	15.29	9015/29	May 2015	Apr 2020
		4257	4530	274	356,200	1,561.8	844 x 162 x 408	15.29	9015/30	May 2015	Apr 2020
		4531	4700	170	221,000	968.0	844 x 162 x 408	9.49	9015/31	May 2015	Apr 2020



Page 1 of 2

a member of admo Group
P.O. Box 30485 Abu Dhabi UAE Tel: +971 2 6199100 Fax: +971 2 5511162 Email: info@admo.ae Web: www.admo.ae

ANNEX 13- INVOICE(SAMPLE)



admd
شركة أبوظبي الطبية والصحية
Abu Dhabi Medical Services Company

COMMERCIAL INVOICE
Invoice No. AD 001-02 / 2017 Dated 06th May 2017

Customer:
UNICEF Supply Division
Purchase / Invoice Certification Unit
UNICEF Plaza - Freeport, DK 2100 Copenhagen OE - Denmark

Tel : + 45 35 27 35 27
Fax : + 45 35 26 84 21

Purchase Order Number: 45125132
UNICEF Material Number: 50782153
Country of Destination: Pakistan via Karachi

Delivery Terms: INCOTERMS 2010
PCA Dubai Seaport Containerized

Reference: LTA 42104709
Supplier Code: 1900010413
Sales Order No.:

Item No.	Description of Contents	Batch / Lot No.	MFG. Date	Expiry Date	Cubic Meters (CBM)	Total No. of Cartons	No. of Boxes per carton	Total No. of Boxes	Unit Price USD	Total Price USD
00010	Syringe, auto-disable, 0.5ml with needle and protective cap, blister packed, box of 100, 0.5ml syringe with fix needle 23G x 1" (0.6mm x 25mm) and protective cap, auto-disable, mixer packed Pre-set volume 1ml with a graduated scale on the barrel, easy to read graduation, two markings: 0 and 0.5ml Brand "MEDECO Inject"	9015/05	May 2015	Apr. 2020	4.30	77	13	1,001	0.0315	3,153.15
		5015/14	Apr. 2015	Mar. 2020	10.04	180	13	2,340	0.0015	7,371.00
		9015/15	Apr. 2015	Mar. 2020	15.29	274	13	3,562	0.0315	11,220.30
		9015/16	Apr. 2015	Mar. 2020	15.29	274	13	3,562	0.0315	11,220.30
		9015/17	Apr. 2015	Mar. 2020	15.29	274	13	3,562	0.0315	11,220.30
		9015/18	Apr. 2015	Mar. 2020	15.29	274	13	3,562	0.0315	11,220.30
		9015/19	Apr. 2015	Mar. 2020	9.10	183	13	2,119	0.0315	6,674.85
		9015/20	Apr. 2015	Mar. 2020	15.29	274	13	3,562	0.0315	11,220.30
		9015/21	Apr. 2015	Mar. 2020	15.29	274	13	3,562	0.0315	11,220.30
		9015/22	Apr. 2015	Mar. 2020	15.29	274	13	3,562	0.0315	11,220.30
		9015/23	Apr. 2015	Mar. 2020	15.29	274	13	3,562	0.0315	11,220.30
		9015/24	Apr. 2015	Mar. 2020	15.29	274	13	3,562	0.0315	11,220.30
		9015/25	Apr. 2015	Mar. 2020	15.29	274	13	3,562	0.0315	11,220.30
		9015/26	Apr. 2015	Mar. 2020	15.29	274	13	3,562	0.0315	11,220.30
		9015/27	Apr. 2015	Mar. 2020	15.29	274	13	3,562	0.0315	11,220.30
		9015/28	Apr. 2015	Mar. 2020	15.29	274	13	3,562	0.0315	11,220.30
		9015/30	May 2015	Apr. 2020	15.29	274	13	3,562	0.0315	11,220.30
		9015/40	May 2015	Apr. 2020	15.29	274	13	3,562	0.0315	11,220.30
		9015/41	May 2015	Apr. 2020	15.29	274	13	3,562	0.0315	11,220.30
		9015/42	May 2015	Apr. 2020	15.29	274	13	3,562	0.0315	11,220.30
		9015/46	May 2015	Apr. 2020	15.29	274	13	3,562	0.0315	11,220.30
		9015/47	May 2015	Apr. 2020	1.12	30	13	280	0.0315	819.00
		9015/48	May 2015	Apr. 2020	15.29	274	13	3,562	0.0315	11,220.30
		9015/50	May 2015	Apr. 2020	15.29	274	13	3,562	0.0315	11,220.30
		9015/52	May 2015	Apr. 2020	15.29	274	13	3,562	0.0315	11,220.30
		9015/53	May 2015	Apr. 2020	15.29	274	13	3,562	0.0315	11,220.30
		9015/54	May 2015	Apr. 2020	15.29	274	13	3,562	0.0315	11,220.30
		9015/55	May 2015	Apr. 2020	15.29	274	13	3,562	0.0315	11,220.30
Total					391.43	7,016		91,208		

Bank Details: HSBC BANK LTD, HSBC A/C No. 001-198629-100, Abu Dhabi, United Arab Emirates.

SWIFT Code: HSBCAG22XXX

Total Gross Weight = 39,991 KG
Total Net Weight = 19,926 KG
Total Volume = 391.43 CBM

Sub Total: 287,305.20

Shipping & Handling:

Discount:

Total PCA Dubai Seaport, Containerized: 287,305.20

1) Container Size (1 x 40' HC) :
2) Container Size (1 x 40' HC) :
3) Container Size (1 x 40' HC) :
4) Container Size (1 x 40' HC) :
5) Container Size (1 x 40' HC) :
6) Container Size (1 x 40' HC) :



ABU DHABI MEDICAL SERVICES CO. LLC

a member of **admd** Group

P O Box 30485 Abu Dhabi UAE Tel: +971 2 6199100 Fax: +971 2 5511162 Email: info@admd.ae Web: www.admd.ae

ANNEX 14- CERTIFICATE OF CONFORMITY (SAMPLE)


admd
Abu Dhabi Medical Devices Company

Certificate No.: 086/QC/CC/0.5ml/15

CERTIFICATE OF CONFORMITY

STERILITY & PACK INTEGRITY

This is to certify that...


Product Description : 0.5 ml Auto Disable Syringe (MEDECO INJECT AD)
Needle Size : 23G x 1" (0.60mm X 25mm)
Product Reference No. : SFG-01003
Purchase Order No. : 45139132
Invoice Reference No. : AD 669-05/2015
UNICEF Material Number : S0782153

Batch Lot No.	Batch Qty	Sterilization Date	Expiry Date
9015/18	231,400 Pcs	April 2015	March 2020
9015/19	211,900 Pcs	April 2015	March 2020
9015/20	356,200 Pcs	April 2015	March 2020
9015/21	356,200 Pcs	April 2015	March 2020
9015/22	356,200 Pcs	April 2015	March 2020
9015/23	15,600 Pcs	April 2015	March 2020

Manufacturing/Sterilization : Abu Dhabi Medical Devices Company, LLC
Abu Dhabi, UAE
Sterilization Method : Ethylene Oxide (90% ETO + 10% CO2)

Is sterilized in accordance with ISO Standard 11135-1 for Sterilization of health care products-ethylene oxide, Requirements for development, validation and routine control of sterilization process for medical devices and with British Standard for Sterilization of Medical Devices as Requirements for terminally – sterilized devices to be labeled "STERILE", BS EN 556-1:2001. The product is tested in accordance with USP and it has passed the Sterility and Endotoxin Level.

Certified Correct
Authorized Person

Sign : 
Name: Mohammed Ahmed Ali
Title : QC Section Head
Date : May 25, 2015

Markings:
45139132
Customer Ref.: PSS – 115-PAK-04A-X/2015
Pakistan via Karachi
GAVI2015-1115-PAK-04A-X/2015

a member of  Group
P.O. Box 30485 Abu Dhabi UAE Tel: +971 2 6199100 Fax: +971 2 5511162 Email: info@admd.ae Web: www.admd.ae

ANNEX 15- PRODUCT ARRIVAL REPORT (SAMPLE)

PRODUCT ARRIVAL REPORT (PAR)

COUNTRY			
REPORT No		Date of report	

Place of inspection	Date and time	Name of store and date and time product entered into store

PART I - ADVANCE NOTICE

Date received by fax/ email	Pre-advice	Copy Airway Bill (AWB) or Bill of Landing (BOL)	Copy Invoice of	Copy of Packing List
	Yes ☐ No ☐	Yes ☐ No ☐	Yes ☐ No ☐	Yes ☐ No ☐

Other documents requested (give description)		Yes ☐ No ☐
--	--	--

PART II - ARRIVAL DETAILS

AWB number or BOL number	Airport/ sea port or border crossing of destination	Flight No Vessel or Vehicle No	ETA as per notification		Actual time of arrival	
			Day	Time	Day	Time

NAME OF CLEARING AGENT: _____ ON BEHALF OF: _____

PART III - DETAILS OF SHIPMENT

Procurement agency	Purchase Order No.	Consignee	Product description	Manufacturer	Country

Product details			
Lot or model number	Number of boxes	Number of items	Expiry date or manufacturing date (as applicable)

(Please continue overleaf if necessary)

Was quantity received as per shipping notification?	Yes ☐ No ☐
If not, were details of short-shipment provided prior to product arrival?	Yes ☐ No ☐

PART IV - DOCUMENTS ACCOMPANYING THE SHIPMENT

Copy of invoice	Copy of packing list	Copy of Certificate of Conformity (where required)	Other (specify)
Yes ☐ No ☐	Yes ☐ No ☐	Yes ☐ No ☐ N/A ☐	Yes ☐ No ☐

PART V - GENERAL CONDITION OF SHIPMENT

What was the condition of boxes on arrival?	
Were necessary labels attached to shipping boxes?	
Other comments:	

--	--

PART VI - NAME AND SIGNATURE

Authorized Inspection Supervisor
Manager

DATE

DATE

Primary

Store

or

FDI



USAID
FROM THE AMERICAN PEOPLE

USAID GLOBAL HEALTH SUPPLY CHAIN PROGRAM
Procurement and Supply Management